

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022681.D
 Acq On : 16 Nov 2022 11:26
 Operator : CG/JU
 Sample : PB149090BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	43	rVB	21823	31824	1.74%	0.152%
2	3.628	106	109	132	rBV	274160	468290	25.56%	2.243%
3	3.958	161	165	171	rVB2	6139	10431	0.57%	0.050%
4	6.993	675	681	684	rBV6	1176	2363	0.13%	0.011%
5	7.046	684	690	704	rVB	374120	581781	31.75%	2.786%
6	7.205	710	717	730	rVB	277351	436008	23.79%	2.088%
7	7.399	744	750	762	rVB	349009	565013	30.83%	2.706%
8	7.875	824	831	843	rVB	266705	430651	23.50%	2.062%
9	8.604	948	955	974	rBV	451461	724319	39.53%	3.469%
10	9.057	1025	1032	1042	rBV	356671	570491	31.13%	2.732%
11	9.781	1149	1155	1166	rBV	302761	496943	27.12%	2.380%
12	10.328	1241	1248	1263	rBV	422212	720925	39.34%	3.452%
13	10.698	1304	1311	1320	rBV	389448	648747	35.40%	3.107%
14	10.851	1329	1337	1351	rBV	431172	754465	41.17%	3.613%
15	12.310	1579	1585	1593	rBV2	4913	8558	0.47%	0.041%
16	13.975	1860	1868	1880	rBV	803944	1100745	60.07%	5.271%
17	14.251	1908	1915	1929	rBV	852883	1247042	68.05%	5.972%
18	14.557	1961	1967	1979	rVB	619818	887323	48.42%	4.249%
19	14.787	2000	2006	2029	rBV	336608	587624	32.07%	2.814%
20	14.928	2029	2030	2035	rVV4	2021	3109	0.17%	0.015%
21	14.981	2035	2039	2044	rVB6	1301	2880	0.16%	0.014%
22	15.557	2130	2137	2149	rBV	1157244	1559957	85.13%	7.470%
23	15.686	2153	2159	2174	rVV	326050	472837	25.80%	2.264%
24	15.798	2174	2178	2183	rVB3	3371	4482	0.24%	0.021%
25	17.316	2430	2436	2444	rBV	710491	1035499	56.51%	4.959%
26	17.422	2447	2454	2470	rVB	1161083	1689208	92.18%	8.089%
27	19.292	2767	2772	2776	rVB3	11511	15393	0.84%	0.074%
28	19.363	2780	2784	2787	rVV2	9822	12551	0.68%	0.060%
29	19.727	2840	2846	2854	rBV	1392671	1832466	100.00%	8.775%
30	21.527	3147	3152	3160	rVB	888270	1113657	60.77%	5.333%
31	23.804	3531	3539	3553	rVB	869546	1826817	99.69%	8.748%
32	23.962	3559	3566	3577	rVB2	508412	1039956	56.75%	4.980%


Sum of corrected areas: 20882355

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022681.D
Acq On : 16 Nov 2022 11:26
Operator : CG/JU
Sample : PB149090BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

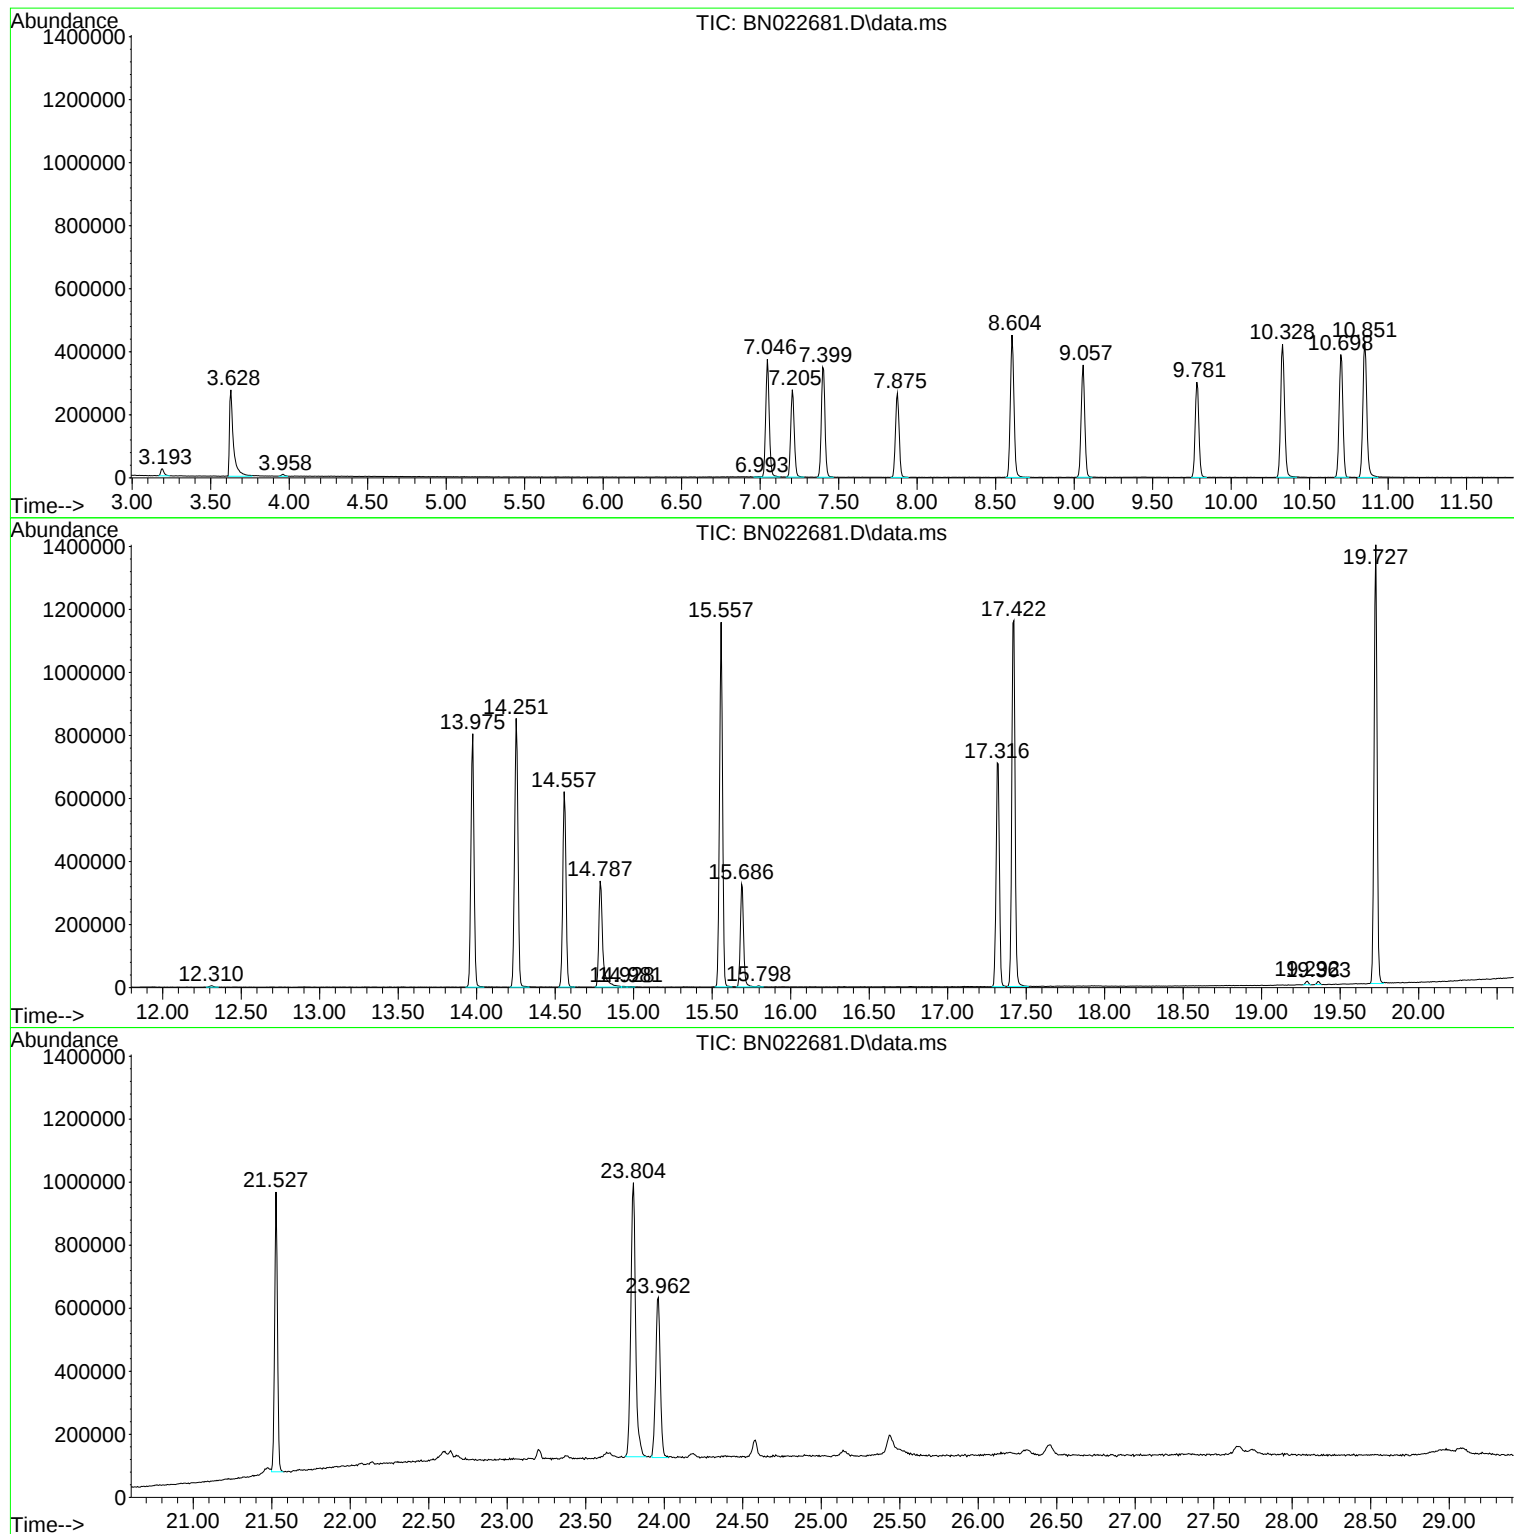

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022681.D
Acq On : 16 Nov 2022 11:26
Operator : CG/JU
Sample : PB149090BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022681.D
Acq On : 16 Nov 2022 11:26
Operator : CG/JU
Sample : PB149090BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc