

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022684.D
 Acq On : 16 Nov 2022 13:16
 Operator : CG/JU
 Sample : N5622-02
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	47	rVB	13876	22310	1.38%	0.144%
2	3.516	87	90	94	rBV5	2091	2893	0.18%	0.019%
3	3.640	109	111	132	rVV	49725	99151	6.15%	0.638%
4	3.858	143	148	156	rVB4	6780	13445	0.83%	0.087%
5	3.958	160	165	170	rBV	8808	12419	0.77%	0.080%
6	4.946	329	333	343	rVB4	2385	5631	0.35%	0.036%
7	5.828	480	483	485	rBV4	1377	1751	0.11%	0.011%
8	5.875	488	491	497	rVB3	1128	1878	0.12%	0.012%
9	7.046	685	690	705	rVB	52688	89673	5.56%	0.577%
10	7.204	710	717	727	rBV	199041	313818	19.45%	2.021%
11	7.399	744	750	761	rBV	192137	310370	19.24%	1.999%
12	7.875	824	831	838	rBV	240562	392415	24.32%	2.527%
13	8.604	949	955	966	rBV	157500	256150	15.88%	1.650%
14	9.057	1025	1032	1044	rBV	252184	414375	25.68%	2.668%
15	9.440	1092	1097	1099	rBV3	1016	1623	0.10%	0.010%
16	9.781	1149	1155	1167	rVB	200015	330792	20.50%	2.130%
17	10.328	1241	1248	1263	rBV	274257	462794	28.68%	2.980%
18	10.698	1303	1311	1320	rBV	359808	587761	36.43%	3.785%
19	10.851	1329	1337	1356	rBV	261852	468163	29.02%	3.015%
20	11.381	1422	1427	1433	rBB5	1047	1810	0.11%	0.012%
21	12.310	1580	1585	1593	rBV2	3155	6013	0.37%	0.039%
22	13.445	1773	1778	1782	rBV2	3667	5675	0.35%	0.037%
23	13.975	1859	1868	1885	rBV	574067	840900	52.12%	5.415%
24	14.251	1908	1915	1933	rBV	660016	931247	57.72%	5.997%
25	14.557	1961	1967	1980	rBV	568460	796731	49.38%	5.131%
26	14.798	2003	2008	2020	rBV2	31096	72570	4.50%	0.467%
27	14.998	2040	2042	2049	rBV4	1391	1675	0.10%	0.011%
28	15.557	2130	2137	2152	rVV	840843	1234177	76.49%	7.948%
29	15.686	2154	2159	2174	rVV	282573	390110	24.18%	2.512%
30	15.792	2174	2177	2181	rVB2	2425	3127	0.19%	0.020%
31	17.316	2430	2436	2447	rBV	671374	946124	58.64%	6.093%
32	17.416	2447	2453	2468	rVB	1044857	1480152	91.74%	9.532%
33	18.210	2585	2588	2594	rBV2	5853	8006	0.50%	0.052%
34	19.286	2767	2771	2778	rVB4	10368	15221	0.94%	0.098%
35	19.357	2780	2783	2789	rBV	8959	12974	0.80%	0.084%
36	19.498	2804	2807	2812	rVV3	6712	8652	0.54%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022684.D
Acq On : 16 Nov 2022 13:16
Operator : CG/JU
Sample : N5622-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	19.645	2830	2832	2835	rVB3	3670	3190	0.20%	0.021%
38	19.727	2840	2846	2860	rVV	1149590	1613433	100.00%	10.390%
39	21.527	3147	3152	3163	rVB	789803	968612	60.03%	6.238%
40	23.798	3532	3538	3551	rVB2	719711	1501371	93.05%	9.668%
41	23.962	3559	3566	3578	rVB	446090	899622	55.76%	5.793%




Sum of corrected areas: 15528804

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022684.D
Acq On : 16 Nov 2022 13:16
Operator : CG/JU
Sample : N5622-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

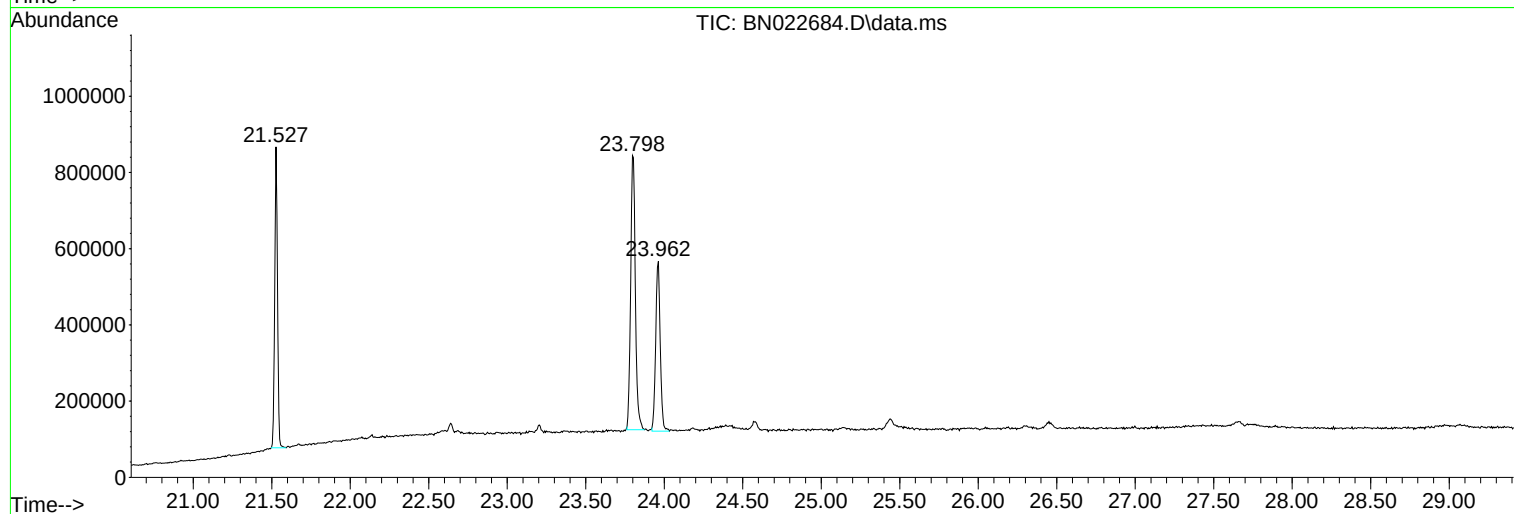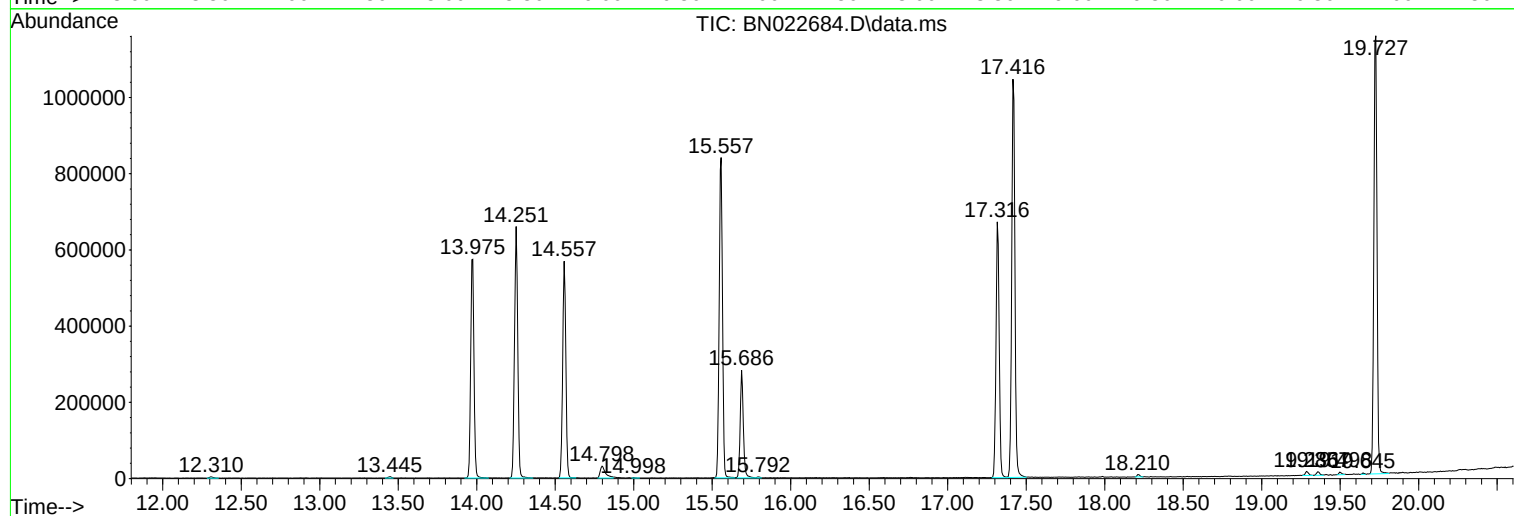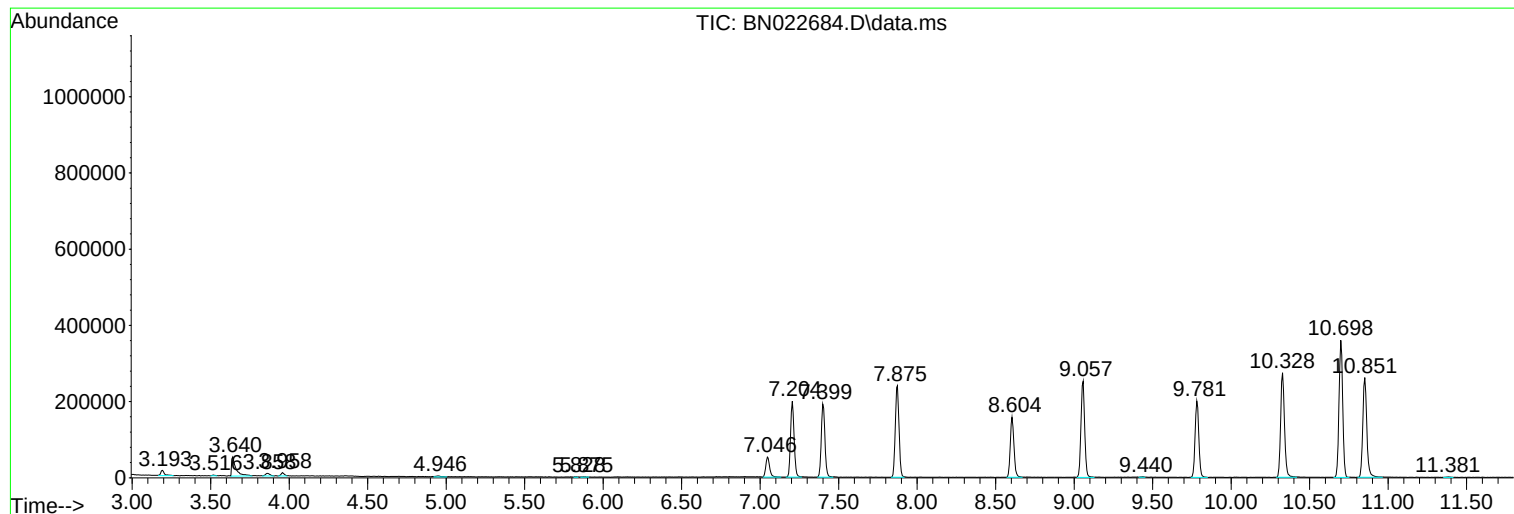

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022684.D
Acq On : 16 Nov 2022 13:16
Operator : CG/JU
Sample : N5622-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022684.D
Acq On : 16 Nov 2022 13:16
Operator : CG/JU
Sample : N5622-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc