

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022687.D
 Acq On : 16 Nov 2022 15:06
 Operator : CG/JU
 Sample : N5622-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	31	rBV4	3644	5044	0.25%	0.027%
2	3.193	31	35	42	rVB	16416	22776	1.11%	0.122%
3	3.505	86	88	95	rBV	3700	6441	0.31%	0.035%
4	3.634	107	110	125	rBV	94333	165198	8.06%	0.888%
5	3.858	144	148	156	rVB2	8264	14653	0.71%	0.079%
6	3.958	161	165	172	rVB	8363	12059	0.59%	0.065%
7	4.952	329	334	337	rBV3	1491	2329	0.11%	0.013%
8	7.046	685	690	702	rVB	75913	124709	6.08%	0.670%
9	7.205	710	717	728	rBV	279806	440690	21.49%	2.369%
10	7.399	744	750	760	rBV	265846	426177	20.78%	2.291%
11	7.875	824	831	839	rVB	255347	413163	20.15%	2.221%
12	8.604	947	955	964	rBV	226335	362168	17.66%	1.947%
13	9.057	1024	1032	1045	rBV	356300	588212	28.69%	3.162%
14	9.781	1149	1155	1164	rBV	240777	393230	19.18%	2.114%
15	10.328	1241	1248	1260	rBV	369828	622215	30.34%	3.344%
16	10.698	1303	1311	1321	rBV	378051	613183	29.90%	3.296%
17	10.851	1330	1337	1352	rBV	380968	672225	32.78%	3.613%
18	12.304	1580	1584	1592	rVB2	4799	8836	0.43%	0.047%
19	13.451	1773	1779	1782	rVB4	1741	2339	0.11%	0.013%
20	13.887	1848	1853	1857	rBV5	1782	2401	0.12%	0.013%
21	13.975	1861	1868	1883	rVV	789267	1119206	54.58%	6.016%
22	14.251	1908	1915	1926	rBV	899631	1263214	61.60%	6.790%
23	14.557	1960	1967	1981	rBV	583362	830178	40.49%	4.462%
24	14.810	2004	2010	2018	rBV3	9950	25521	1.24%	0.137%
25	15.557	2130	2137	2147	rBV	1147456	1619629	78.99%	8.705%
26	15.692	2156	2160	2169	rVB2	15548	22822	1.11%	0.123%
27	15.792	2173	2177	2181	rBV4	3411	4592	0.22%	0.025%
28	17.316	2430	2436	2447	rBV	680247	976169	47.61%	5.247%
29	17.416	2447	2453	2469	rVV	1288510	1902439	92.78%	10.226%
30	17.528	2469	2472	2474	rVB4	2656	2897	0.14%	0.016%
31	19.286	2767	2771	2776	rVB	13966	18722	0.91%	0.101%
32	19.357	2779	2783	2789	rBV	11697	17199	0.84%	0.092%
33	19.645	2830	2832	2836	rVB5	2838	2978	0.15%	0.016%
34	19.727	2839	2846	2856	rVV	1526889	2050526	100.00%	11.021%
35	19.957	2882	2885	2891	rVB3	11162	12273	0.60%	0.066%
36	21.527	3147	3152	3160	rVB	781211	999700	48.75%	5.373%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022687.D
Acq On : 16 Nov 2022 15:06
Operator : CG/JU
Sample : N5622-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.804	3531	3539	3552	rVB2	901289	1925740	93.91%	10.351%
38	23.962	3559	3566	3579	rVB2	465341	912962	44.52%	4.907%




Sum of corrected areas: 18604815

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022687.D
Acq On : 16 Nov 2022 15:06
Operator : CG/JU
Sample : N5622-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

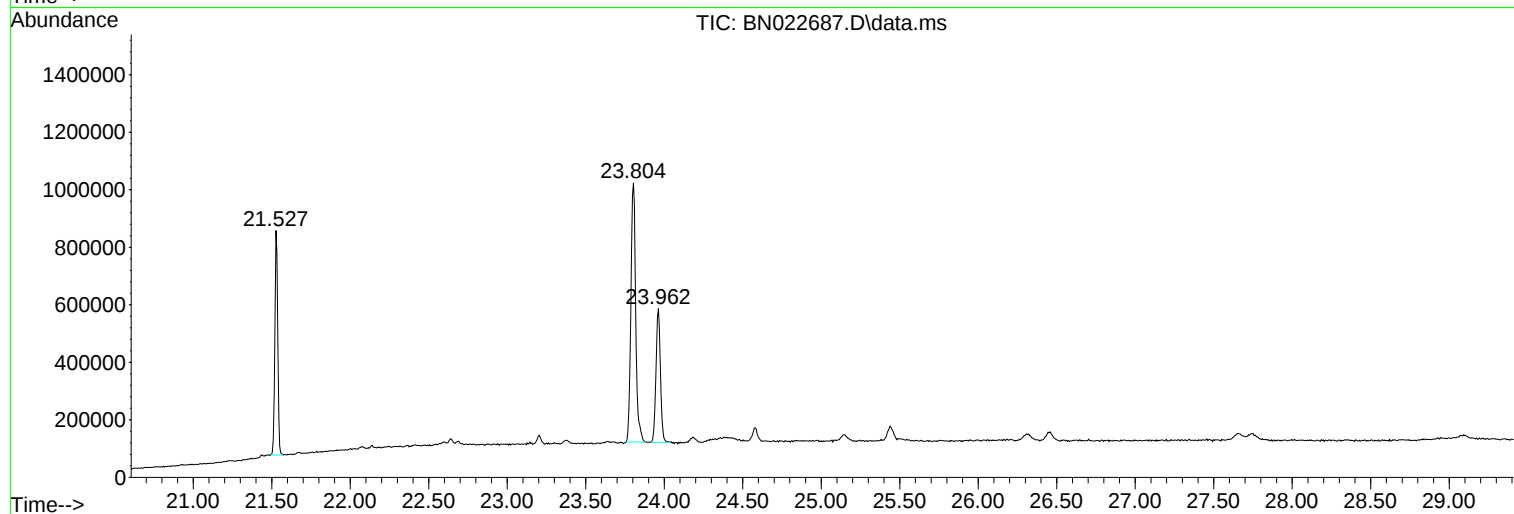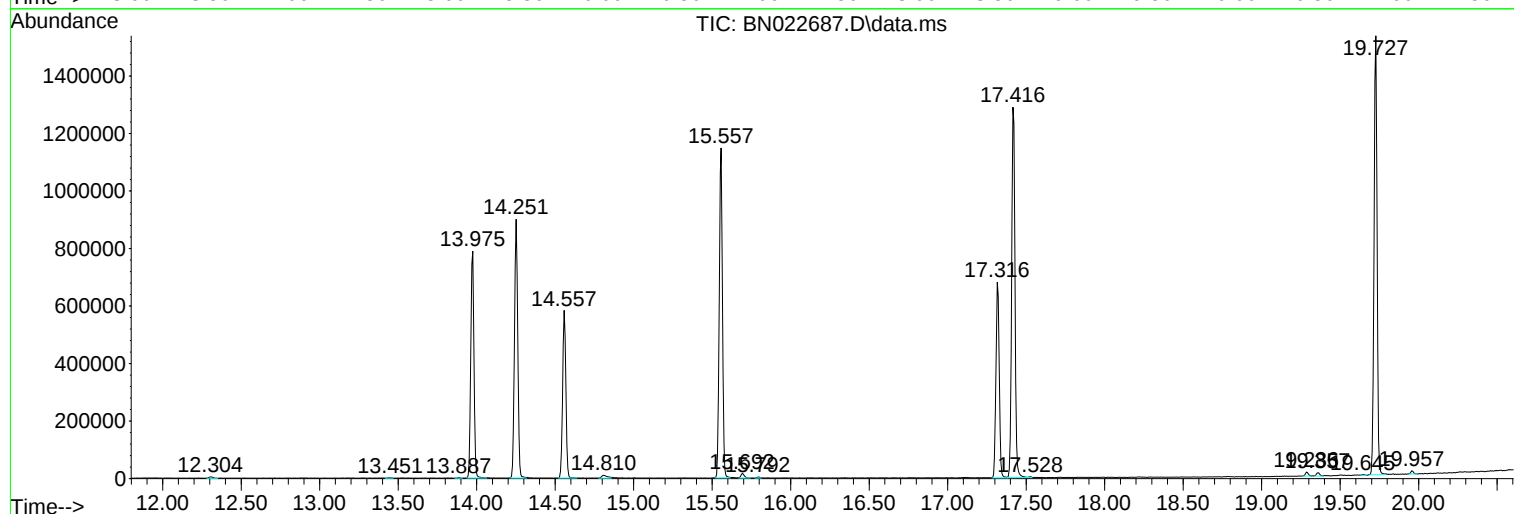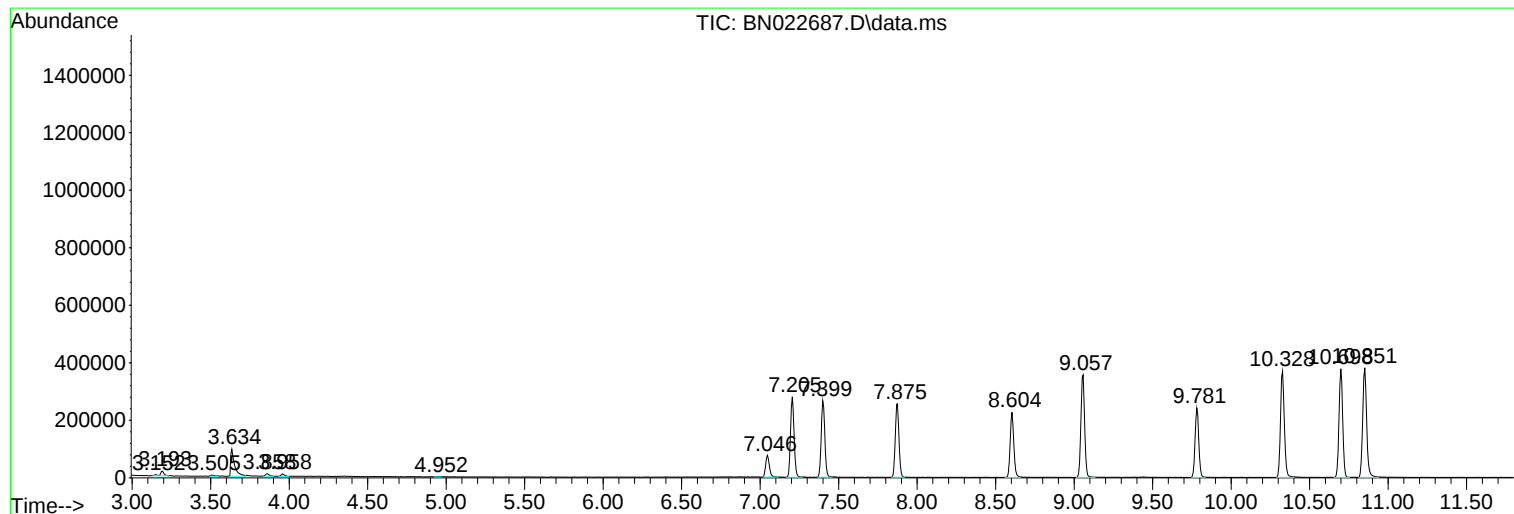

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022687.D
Acq On : 16 Nov 2022 15:06
Operator : CG/JU
Sample : N5622-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022687.D
Acq On : 16 Nov 2022 15:06
Operator : CG/JU
Sample : N5622-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
