

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022694.D
 Acq On : 16 Nov 2022 19:26
 Operator : CG/JU
 Sample : PB149092BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	27500	41953	1.88%	0.163%
2	3.628	106	109	127	rBV	337011	574344	25.76%	2.232%
3	3.958	161	165	170	rBV	6125	8623	0.39%	0.034%
4	7.046	683	690	709	rBV	448912	719121	32.25%	2.795%
5	7.205	710	717	727	rBV	351487	536064	24.04%	2.084%
6	7.399	744	750	764	rVB	427953	697882	31.30%	2.712%
7	7.875	824	831	845	rVB	336475	553934	24.84%	2.153%
8	8.605	948	955	969	rBV	550277	890972	39.96%	3.463%
9	9.057	1021	1032	1045	rBV	439451	709307	31.81%	2.757%
10	9.781	1147	1155	1167	rBV	376958	614298	27.55%	2.388%
11	10.322	1241	1247	1258	rBV	513306	881691	39.54%	3.427%
12	10.699	1304	1311	1319	rBV	501758	823144	36.91%	3.199%
13	10.852	1329	1337	1360	rBV	523112	935814	41.97%	3.637%
14	12.304	1577	1584	1593	rBV	5462	10704	0.48%	0.042%
15	13.975	1855	1868	1881	rBV	965717	1337183	59.97%	5.197%
16	14.251	1908	1915	1924	rBV	1092336	1520995	68.21%	5.912%
17	14.557	1960	1967	1977	rBV	775044	1110369	49.80%	4.316%
18	14.787	1999	2006	2023	rBV	410072	726399	32.58%	2.823%
19	15.557	2130	2137	2149	rBV	1295861	1879681	84.30%	7.306%
20	15.687	2154	2159	2173	rVV	434059	599860	26.90%	2.331%
21	15.792	2173	2177	2183	rVB	5389	7399	0.33%	0.029%
22	17.104	2396	2400	2403	rBV3	1611	2315	0.10%	0.009%
23	17.316	2430	2436	2447	rBV	919513	1309502	58.73%	5.090%
24	17.416	2447	2453	2466	rBV	1452141	2053749	92.10%	7.982%
25	19.286	2767	2771	2777	rVB	13938	19396	0.87%	0.075%
26	19.357	2779	2783	2790	rVV	14026	19168	0.86%	0.075%
27	19.728	2839	2846	2861	rBV	1590943	2222666	99.68%	8.639%
28	21.527	3147	3152	3161	rBV	1071145	1363864	61.16%	5.301%
29	23.804	3531	3539	3553	rVB2	1025789	2229848	100.00%	8.667%
30	23.957	3558	3565	3576	rVB2	655418	1328385	59.57%	5.163%


Sum of corrected areas: 25728630

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022694.D
Acq On : 16 Nov 2022 19:26
Operator : CG/JU
Sample : PB149092BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

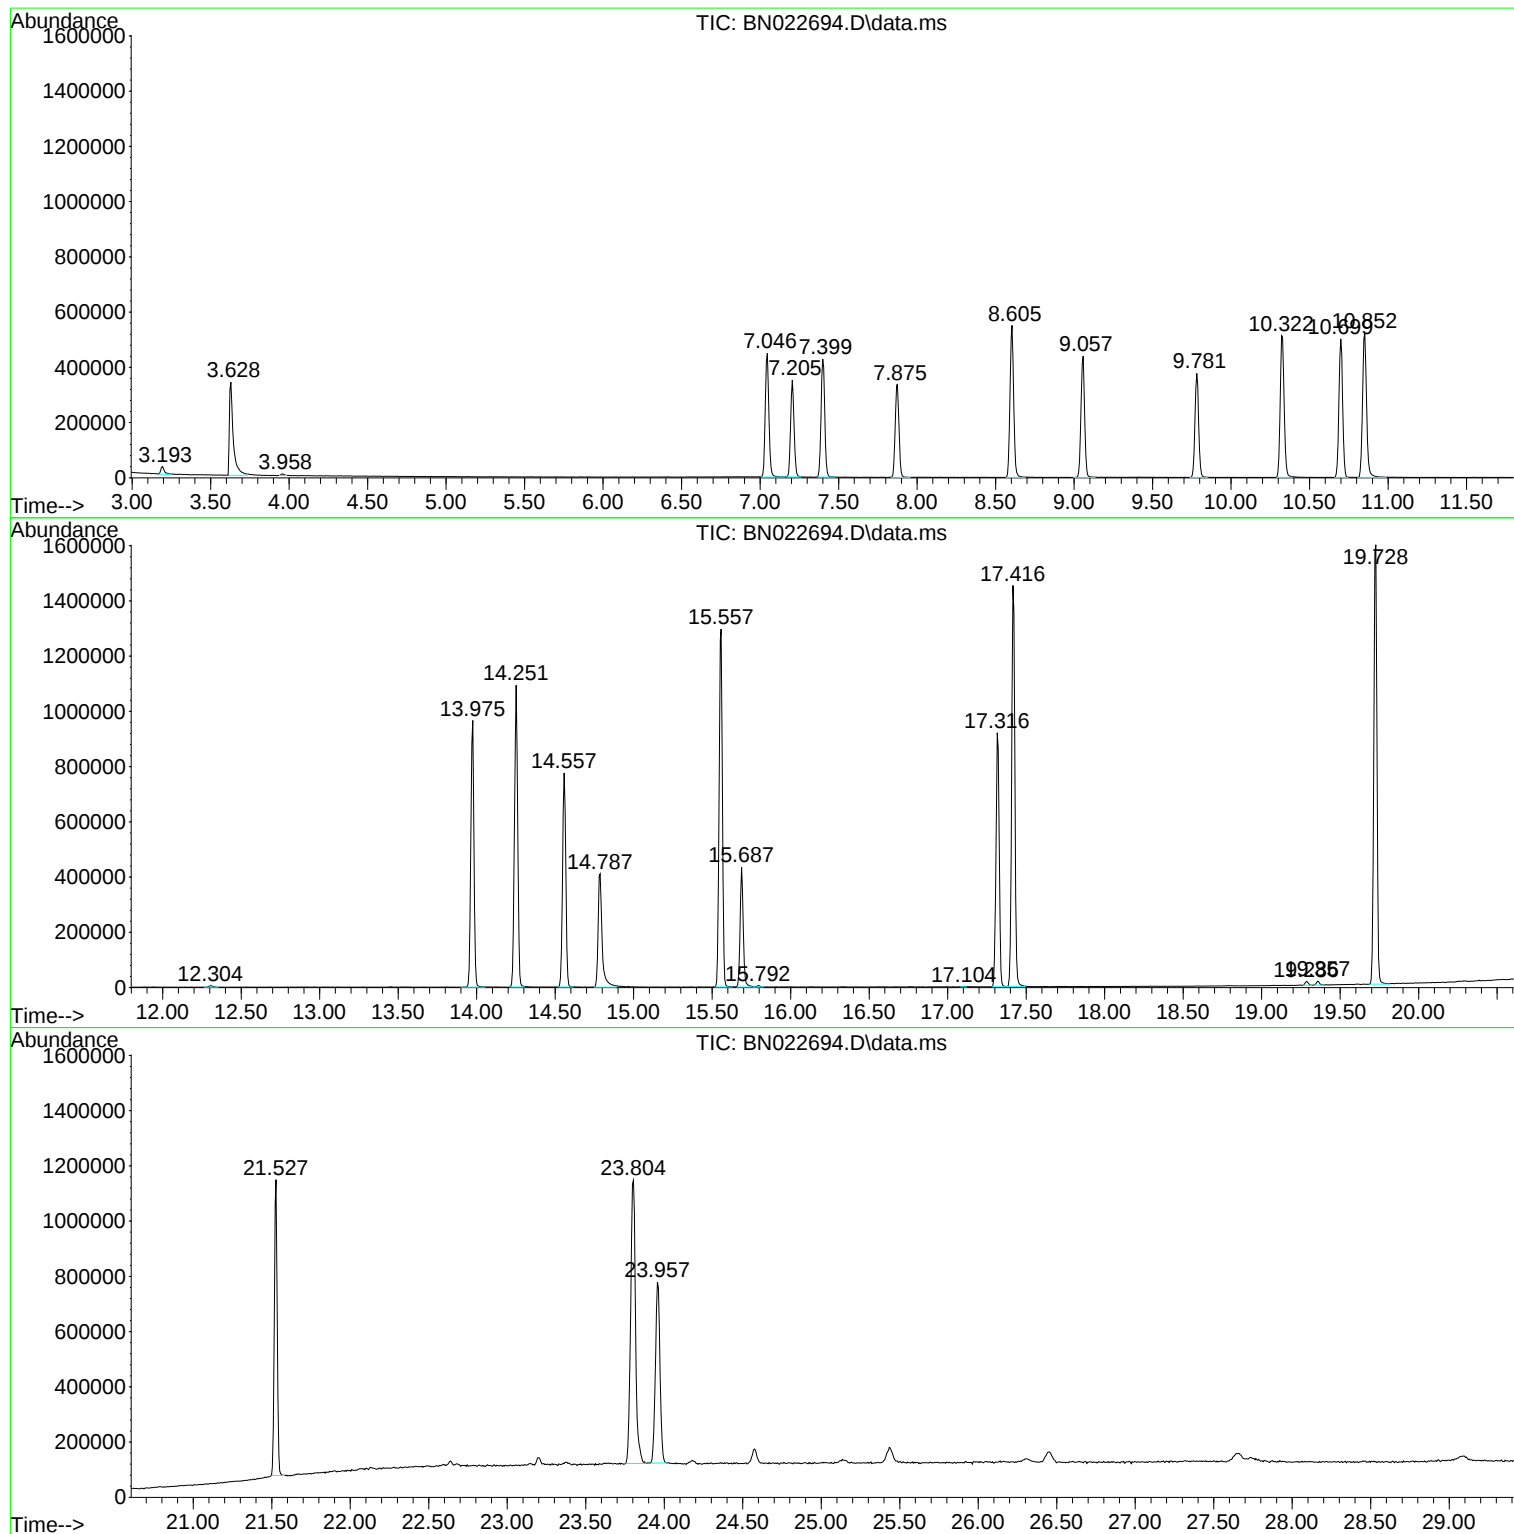

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022694.D
Acq On : 16 Nov 2022 19:26
Operator : CG/JU
Sample : PB149092BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022694.D
Acq On : 16 Nov 2022 19:26
Operator : CG/JU
Sample : PB149092BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc