

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022698.D
 Acq On : 16 Nov 2022 22:30
 Operator : CG/JU
 Sample : PB148999BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK999

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	44	rVB	25756	40386	1.95%	0.176%
2	3.628	105	109	134	rBV	301104	507339	24.51%	2.216%
3	3.958	162	165	170	rVB3	6416	9372	0.45%	0.041%
4	7.040	683	689	703	rBV	416029	681173	32.91%	2.975%
5	7.205	710	717	727	rBV	329172	507104	24.50%	2.215%
6	7.399	743	750	763	rBV	409011	658558	31.82%	2.876%
7	7.869	824	830	840	rBV	305700	481977	23.29%	2.105%
8	8.599	948	954	969	rBV	506271	836872	40.43%	3.655%
9	9.052	1024	1031	1045	rBV	404984	665093	32.13%	2.905%
10	9.781	1148	1155	1166	rVB	355696	575189	27.79%	2.512%
11	10.322	1240	1247	1260	rBV	495461	834088	40.30%	3.643%
12	10.699	1303	1311	1318	rBV	433098	715741	34.58%	3.126%
13	10.846	1328	1336	1357	rBV	401244	738444	35.68%	3.225%
14	12.304	1579	1584	1593	rVB3	5366	10317	0.50%	0.045%
15	13.446	1774	1778	1782	rBV2	1548	2528	0.12%	0.011%
16	13.969	1861	1867	1880	rBV	862012	1232023	59.53%	5.381%
17	14.251	1908	1915	1931	rBV	956439	1411961	68.22%	6.166%
18	14.557	1960	1967	1976	rBV	673715	964254	46.59%	4.211%
19	14.781	1999	2005	2034	rBV	370689	654243	31.61%	2.857%
20	15.551	2130	2136	2144	rBV	1208367	1755664	84.82%	7.667%
21	15.687	2153	2159	2171	rBV	391063	536242	25.91%	2.342%
22	15.793	2174	2177	2181	rVB2	4834	5800	0.28%	0.025%
23	17.104	2395	2400	2401	rBV4	1778	2477	0.12%	0.011%
24	17.316	2430	2436	2446	rBV	793334	1112320	53.74%	4.858%
25	17.416	2446	2453	2470	rVB	1400853	1922807	92.90%	8.397%
26	19.286	2767	2771	2776	rVB3	14280	17851	0.86%	0.078%
27	19.357	2779	2783	2789	rBV	12452	17268	0.83%	0.075%
28	19.498	2805	2807	2809	rBV3	1989	2118	0.10%	0.009%
29	19.722	2839	2845	2857	rVV	1516038	2069751	100.00%	9.039%
30	21.528	3147	3152	3158	rVB	870904	1112600	53.76%	4.859%
31	23.798	3531	3538	3554	rVB2	870453	1832118	88.52%	8.001%
32	23.957	3558	3565	3581	rVB2	457272	983877	47.54%	4.297%


Sum of corrected areas: 22897555

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022698.D
Acq On : 16 Nov 2022 22:30
Operator : CG/JU
Sample : PB148999BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

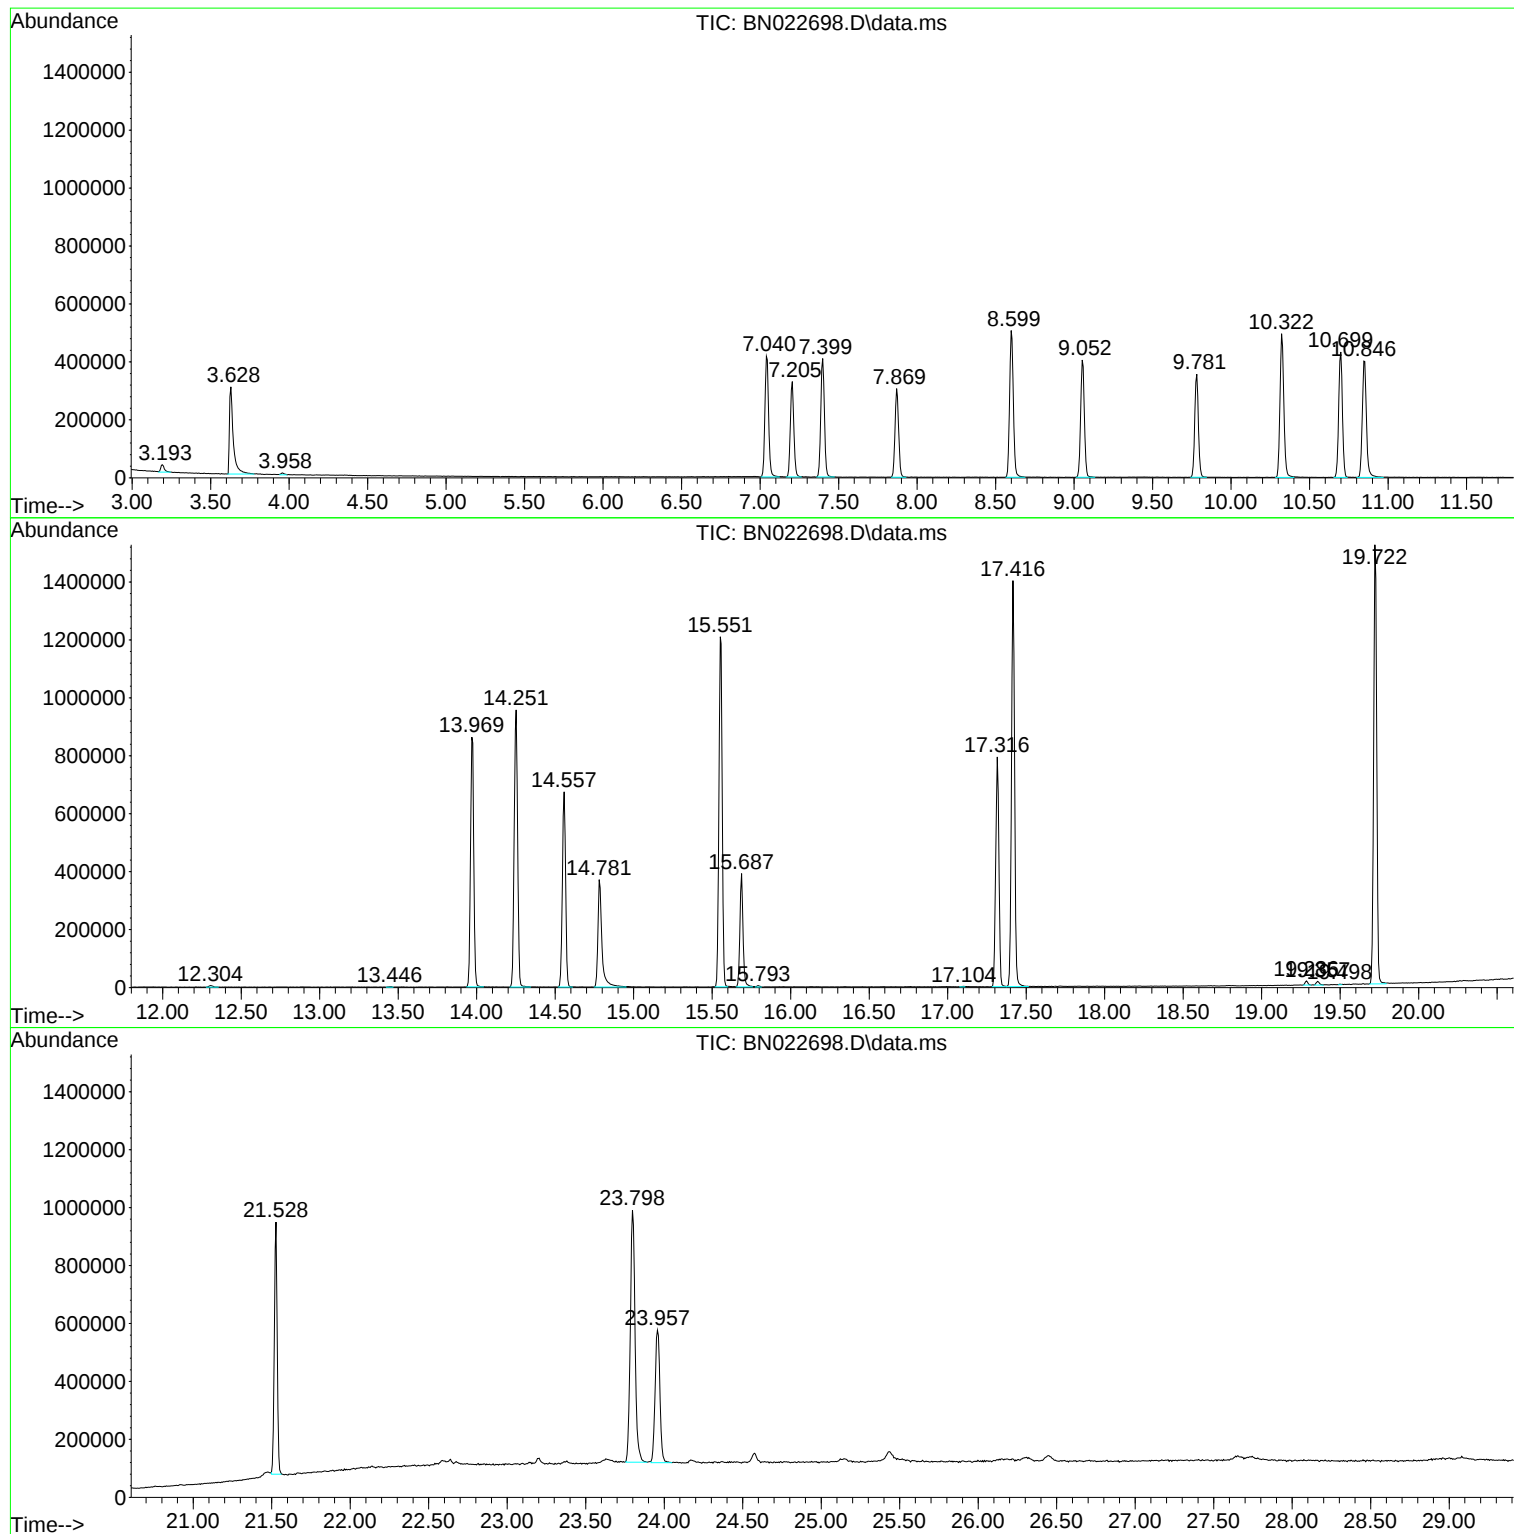

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022698.D
Acq On : 16 Nov 2022 22:30
Operator : CG/JU
Sample : PB148999BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022698.D
Acq On : 16 Nov 2022 22:30
Operator : CG/JU
Sample : PB148999BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK999

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc