

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022699.D
 Acq On : 16 Nov 2022 23:07
 Operator : CG/JU
 Sample : PB149001BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	29706	44211	1.98%	0.180%
2	3.628	106	109	132	rBV	331685	553140	24.73%	2.256%
3	3.958	162	165	169	rVB3	4762	6179	0.28%	0.025%
4	7.040	683	689	703	rBV	459993	735617	32.89%	3.000%
5	7.205	710	717	727	rBV	350927	548169	24.51%	2.235%
6	7.399	743	750	759	rBV	456609	717002	32.06%	2.924%
7	7.869	824	830	840	rVB	307159	486177	21.74%	1.983%
8	8.599	948	954	970	rVB	558127	907307	40.57%	3.700%
9	9.052	1024	1031	1043	rBV	441088	722564	32.31%	2.946%
10	9.781	1148	1155	1165	rBV	387318	629985	28.17%	2.569%
11	10.322	1240	1247	1264	rBV	547624	908521	40.62%	3.705%
12	10.699	1302	1311	1319	rBV	438841	723169	32.34%	2.949%
13	10.846	1328	1336	1357	rBV	437533	795422	35.57%	3.244%
14	12.310	1578	1585	1591	rBV2	5232	10358	0.46%	0.042%
15	13.451	1772	1779	1783	rVB3	1848	3232	0.14%	0.013%
16	13.969	1861	1867	1881	rVB	946140	1322339	59.13%	5.392%
17	14.251	1908	1915	1927	rBV	1041181	1526514	68.26%	6.225%
18	14.557	1960	1967	1979	rBV	674857	968756	43.32%	3.950%
19	14.781	1999	2005	2025	rBV	420382	714133	31.93%	2.912%
20	15.557	2130	2137	2145	rBV	1335461	1877945	83.97%	7.658%
21	15.687	2153	2159	2173	rBV	429259	598866	26.78%	2.442%
22	15.793	2173	2177	2181	rVB	5303	6795	0.30%	0.028%
23	17.104	2396	2400	2403	rBV4	1425	2320	0.10%	0.009%
24	17.316	2430	2436	2447	rBV	797608	1116299	49.92%	4.552%
25	17.416	2447	2453	2469	rVV	1465072	2064615	92.32%	8.419%
26	17.604	2480	2485	2488	rBV5	1358	2250	0.10%	0.009%
27	19.169	2750	2751	2755	rBV3	1752	2301	0.10%	0.009%
28	19.286	2767	2771	2776	rBV2	14154	18717	0.84%	0.076%
29	19.357	2779	2783	2789	rBV2	13085	17950	0.80%	0.073%
30	19.722	2839	2845	2854	rBV	1603441	2236378	100.00%	9.119%
31	21.522	3146	3151	3161	rBV	844230	1164679	52.08%	4.749%
32	23.798	3531	3538	3552	rVB	1001061	2057180	91.99%	8.389%
33	23.957	3558	3565	3577	rVB2	494312	1034169	46.24%	4.217%


Sum of corrected areas: 24523259

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022699.D
Acq On : 16 Nov 2022 23:07
Operator : CG/JU
Sample : PB149001BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

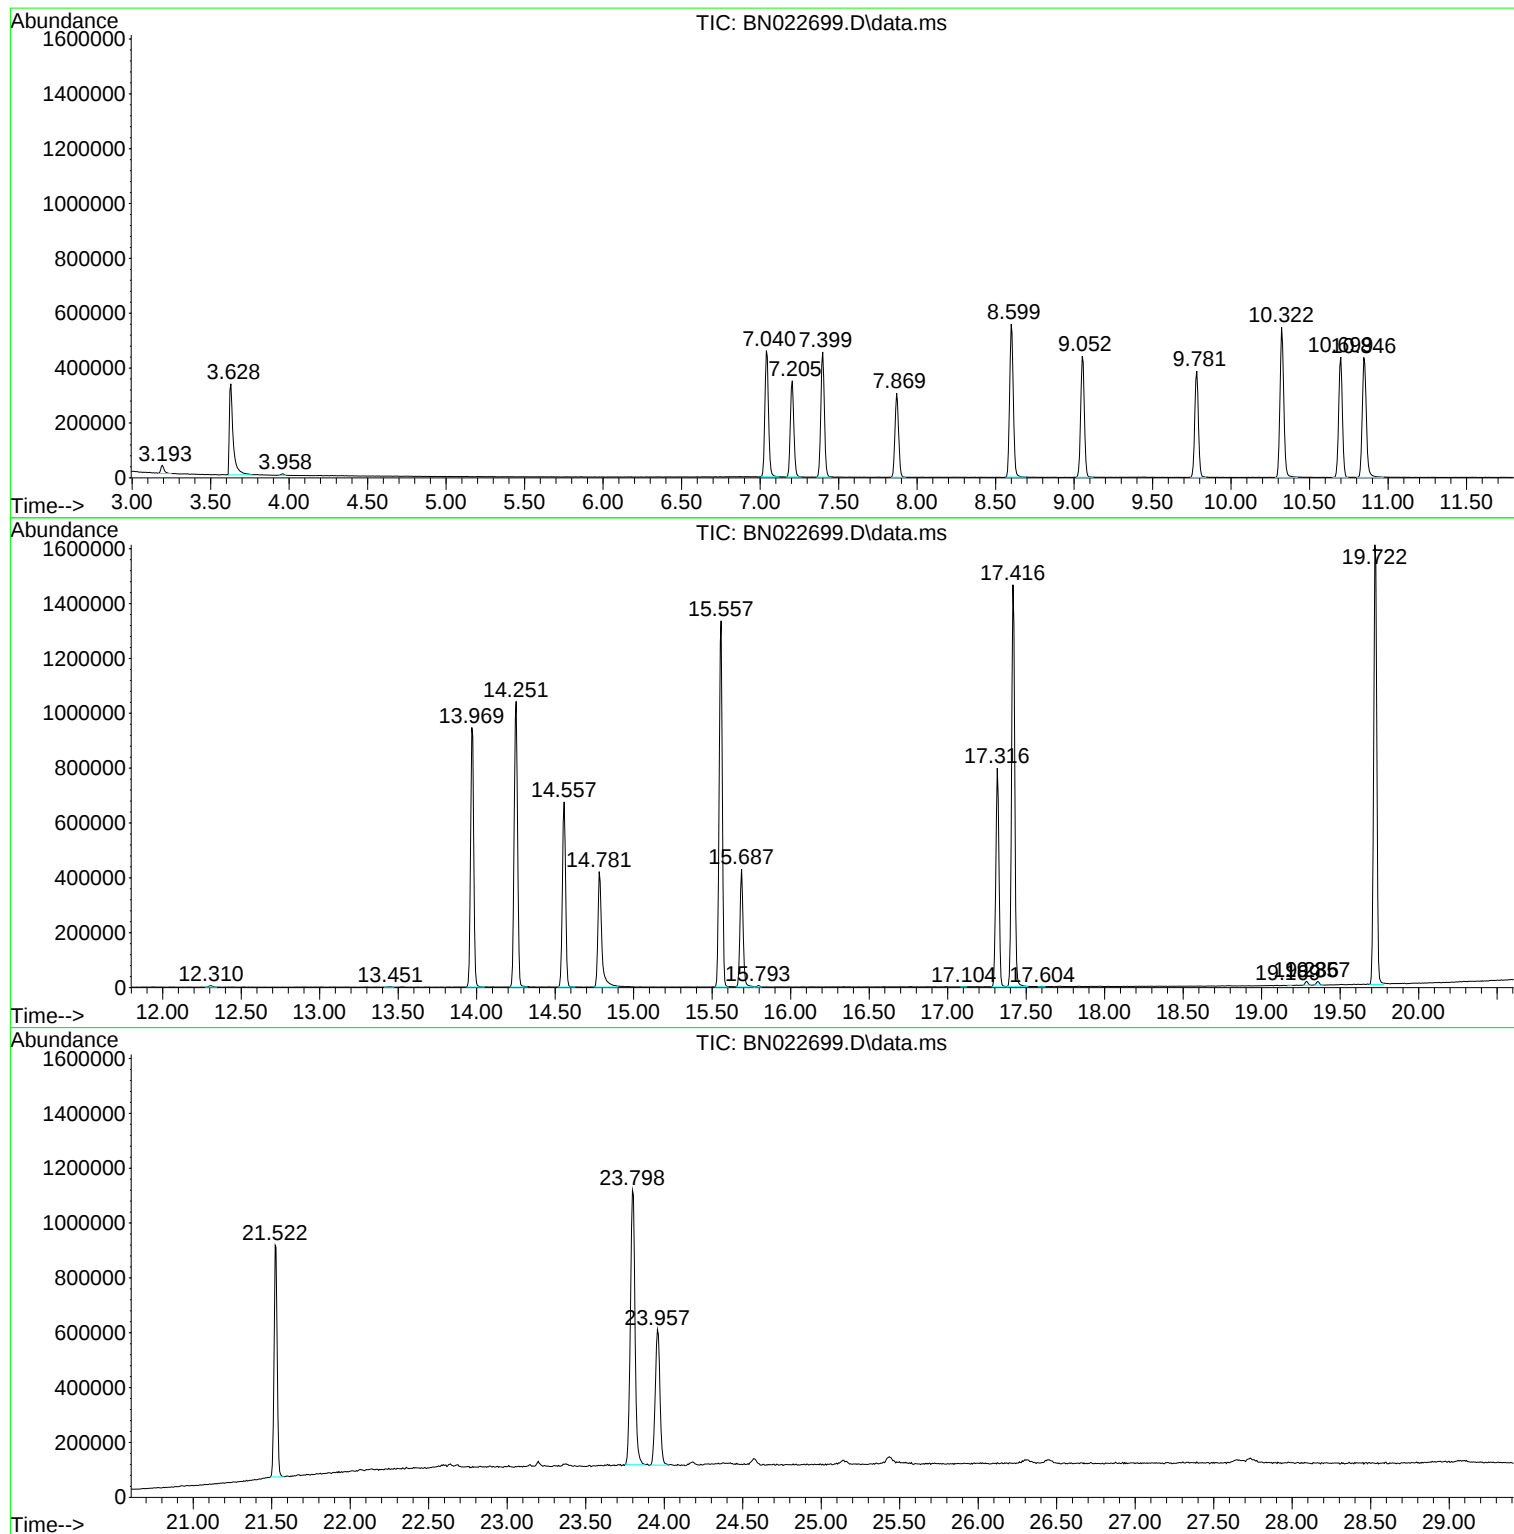

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022699.D
Acq On : 16 Nov 2022 23:07
Operator : CG/JU
Sample : PB149001BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022699.D
Acq On : 16 Nov 2022 23:07
Operator : CG/JU
Sample : PB149001BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK001

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc