

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022704.D
 Acq On : 17 Nov 2022 02:10
 Operator : CG/JU
 Sample : N5577-05
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	40	rBV	17426	23539	1.12%	0.112%
2	3.634	107	110	126	rBV	84696	151878	7.25%	0.725%
3	3.858	143	148	153	rVB2	7605	13336	0.64%	0.064%
4	3.958	161	165	174	rVB2	5886	8826	0.42%	0.042%
5	4.993	334	341	345	rBV5	1100	2936	0.14%	0.014%
6	7.040	684	689	699	rBV	85867	140145	6.69%	0.669%
7	7.205	710	717	727	rBV	285697	460112	21.97%	2.198%
8	7.399	743	750	761	rBV	287891	465895	22.25%	2.225%
9	7.469	761	762	767	rVB3	2294	2499	0.12%	0.012%
10	7.869	824	830	844	rVB	313566	493091	23.55%	2.355%
11	8.599	947	954	965	rBV	225892	371350	17.73%	1.774%
12	9.052	1024	1031	1041	rBV	371461	609126	29.09%	2.909%
13	9.781	1148	1155	1164	rBV	301329	495043	23.64%	2.365%
14	9.910	1173	1177	1182	rBV4	3093	5350	0.26%	0.026%
15	9.963	1182	1186	1194	rVB3	1848	3952	0.19%	0.019%
16	10.322	1240	1247	1268	rBV	404024	699704	33.41%	3.342%
17	10.481	1268	1274	1290	rBV2	23335	57371	2.74%	0.274%
18	10.693	1303	1310	1321	rVB	442918	738949	35.29%	3.530%
19	10.846	1329	1336	1351	rBV	229957	405545	19.37%	1.937%
20	11.493	1441	1446	1454	rBV4	8458	17865	0.85%	0.085%
21	12.298	1579	1583	1589	rVB3	5254	8988	0.43%	0.043%
22	13.157	1725	1729	1735	rVB2	2168	3353	0.16%	0.016%
23	13.440	1773	1777	1784	rVB	9621	15545	0.74%	0.074%
24	13.722	1820	1825	1830	rBV2	2770	4769	0.23%	0.023%
25	13.769	1830	1833	1838	rVV2	4349	6891	0.33%	0.033%
26	13.822	1841	1842	1848	rVB5	1905	2434	0.12%	0.012%
27	13.969	1855	1867	1878	rBV	886643	1201242	57.36%	5.738%
28	14.210	1902	1908	1909	rBV	38009	45966	2.19%	0.220%
29	14.245	1909	1914	1922	rVV	884831	1322273	63.14%	6.316%
30	14.340	1926	1930	1937	rVV	23287	32876	1.57%	0.157%
31	14.440	1941	1947	1952	rVB8	1419	2570	0.12%	0.012%
32	14.557	1960	1967	1976	rBV	685420	1001178	47.81%	4.782%
33	14.787	2000	2006	2027	rBV	58290	131644	6.29%	0.629%
34	14.969	2033	2037	2041	rBV3	2079	2664	0.13%	0.013%
35	15.345	2094	2101	2104	rBV	4949	7018	0.34%	0.034%
36	15.387	2104	2108	2113	rVB3	3002	5751	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022704.D
 Acq On : 17 Nov 2022 02:10
 Operator : CG/JU
 Sample : N5577-05
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	15.551	2129	2136	2143	rBV	1170340	1665962	79.55%	7.957%
38	15.610	2143	2146	2149	rVV3	7318	9434	0.45%	0.045%
39	15.687	2153	2159	2173	rVV	431714	624555	29.82%	2.983%
40	15.792	2173	2177	2181	rVB3	4335	6005	0.29%	0.029%
41	15.951	2202	2204	2208	rVB3	2338	2479	0.12%	0.012%
42	16.122	2226	2233	2237	rBV4	1433	3274	0.16%	0.016%
43	16.275	2253	2259	2265	rBV7	3991	7960	0.38%	0.038%
44	16.339	2265	2270	2273	rVB3	2547	4023	0.19%	0.019%
45	16.445	2282	2288	2292	rVB5	3434	5950	0.28%	0.028%
46	17.063	2387	2393	2396	rBV2	4078	6007	0.29%	0.029%
47	17.104	2396	2400	2404	rBV3	2606	3874	0.18%	0.019%
48	17.228	2417	2421	2425	rVB3	7997	8285	0.40%	0.040%
49	17.316	2429	2436	2444	rBV	840443	1183074	56.49%	5.651%
50	17.416	2447	2453	2464	rVV2	1252515	1770815	84.56%	8.458%
51	17.616	2483	2487	2491	rVB4	3383	4292	0.20%	0.021%
52	17.804	2515	2519	2523	rBV3	3496	4624	0.22%	0.022%
53	17.986	2546	2550	2553	rBV2	9799	11450	0.55%	0.055%
54	18.086	2563	2567	2577	rBV10	2207	4097	0.20%	0.020%
55	18.210	2582	2588	2593	rBV	46644	62040	2.96%	0.296%
56	18.286	2599	2601	2604	rBV	2168	2173	0.10%	0.010%
57	18.504	2634	2638	2642	rBV5	3966	6103	0.29%	0.029%
58	18.569	2644	2649	2650	rBV4	2754	4184	0.20%	0.020%
59	18.716	2671	2674	2679	rBV3	10630	14348	0.69%	0.069%
60	18.963	2714	2716	2720	rVB5	2621	3340	0.16%	0.016%
61	19.286	2765	2771	2774	rBV	17349	24313	1.16%	0.116%
62	19.357	2779	2783	2794	rVB	19736	34932	1.67%	0.167%
63	19.498	2802	2807	2813	rBV3	30439	43575	2.08%	0.208%
64	19.645	2829	2832	2836	rBV6	5328	6666	0.32%	0.032%
65	19.722	2839	2845	2851	rBV2	1566163	2094206	100.00%	10.003%
66	21.227	3098	3101	3109	rBV5	25212	53749	2.57%	0.257%
67	21.522	3146	3151	3160	rVB	908779	1200998	57.35%	5.737%
68	23.798	3530	3538	3554	rVB2	949369	2005085	95.74%	9.577%
69	23.957	3558	3565	3580	rVB2	517310	1092502	52.17%	5.218%




Sum of corrected areas: 20936048

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022704.D
Acq On : 17 Nov 2022 02:10
Operator : CG/JU
Sample : N5577-05
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

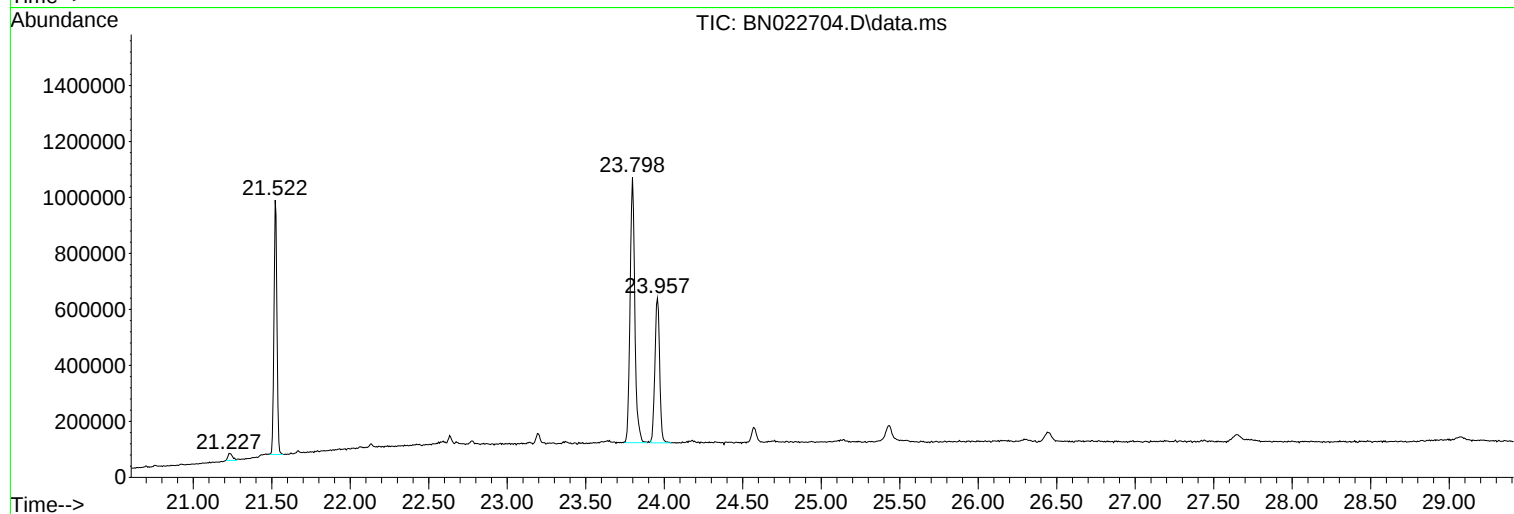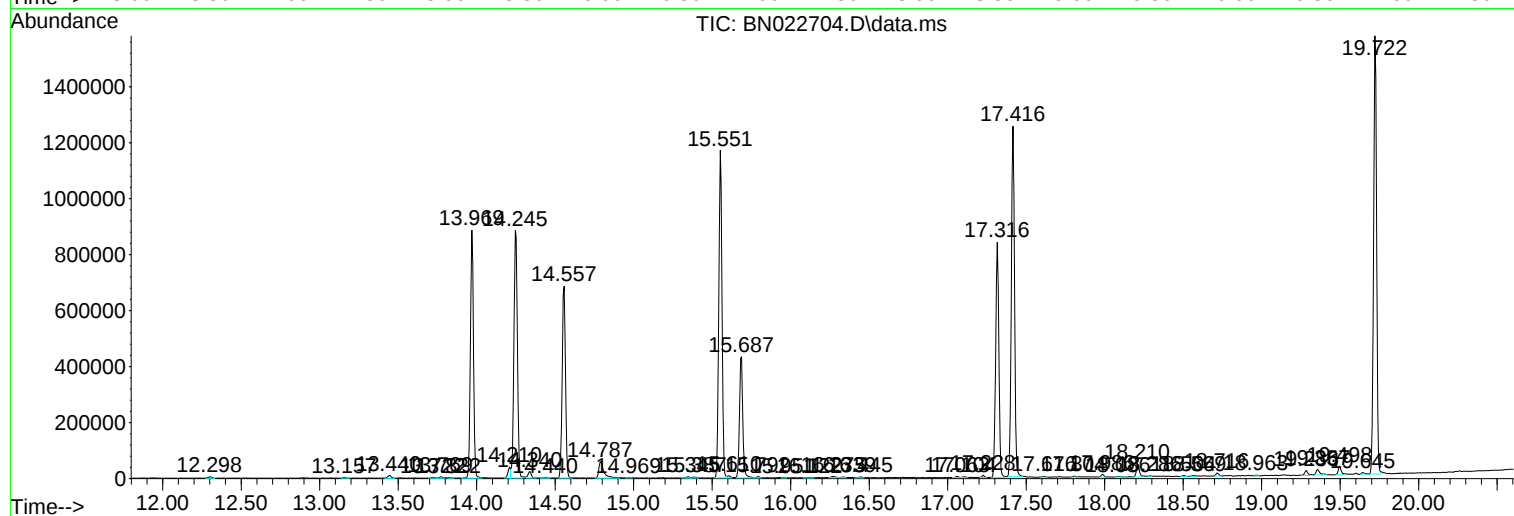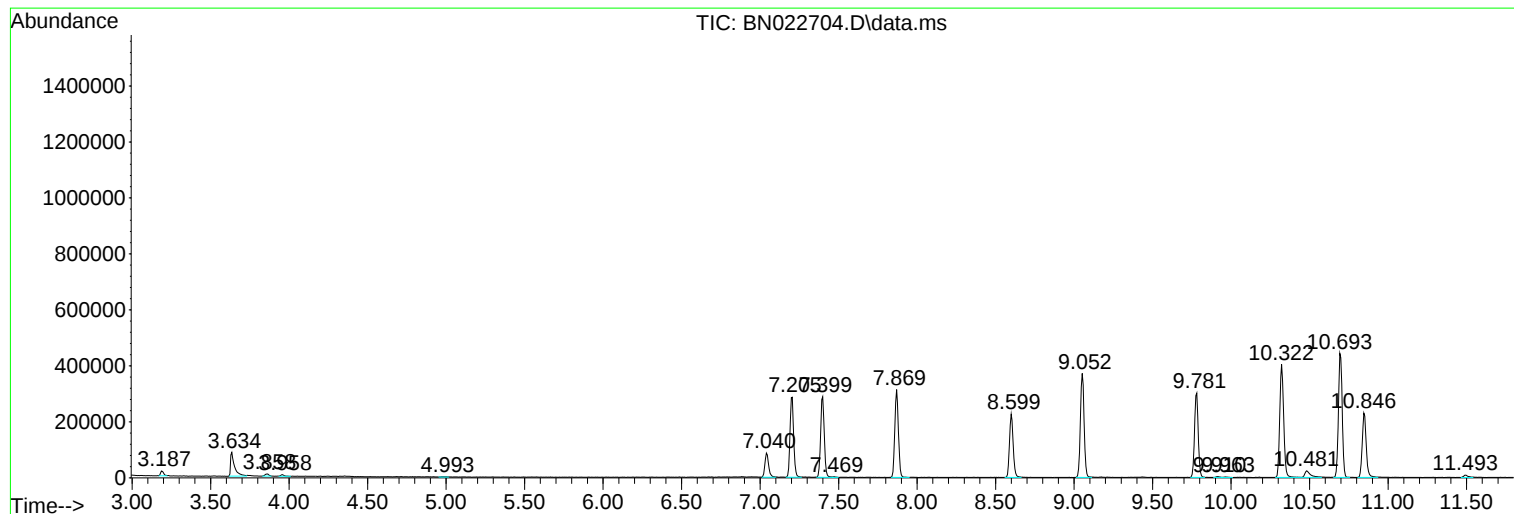

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022704.D
Acq On : 17 Nov 2022 02:10
Operator : CG/JU
Sample : N5577-05
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022704.D
Acq On : 17 Nov 2022 02:10
Operator : CG/JU
Sample : N5577-05
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
