

Data File : BN003573.D
Acq On : 16 Nov 2018 20:43
Operator : MJ/SJ
Sample : J5928-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z2

Quant Time: Nov 16 22:21:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	104847	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	472821	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	285953	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	582994	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	706187	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	772190	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	2697	1.22	ng/uL	0.00
5) Phenol-d5	6.99	99	55336	6.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	137781	28.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	167384	22.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	102582	14.09	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	99809	27.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	114209	28.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	193748	24.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	364	0.05	ng/ul	-0.14
43) Dimethylphthalate-d6	13.88	166	673986	28.43	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	804433	27.28	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	23327	4.91	ng/ul	0.00
57) Fluorene-d10	15.47	176	557942	28.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	94685	23.12	ng/ul	0.00
70) Anthracene-d10	17.32	188	807409	28.19	ng/ul	0.00
78) Pyrene-d10	19.61	212	964326	27.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	1178580	28.19	ng/ul	0.00


Target Compounds					Qvalue	
6) Phenol	7.02	94	15238	1.748	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003573.D
Acq On : 16 Nov 2018 20:43
Operator : MJ/SJ
Sample : J5928-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z2

Quant Time: Nov 16 22:21:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

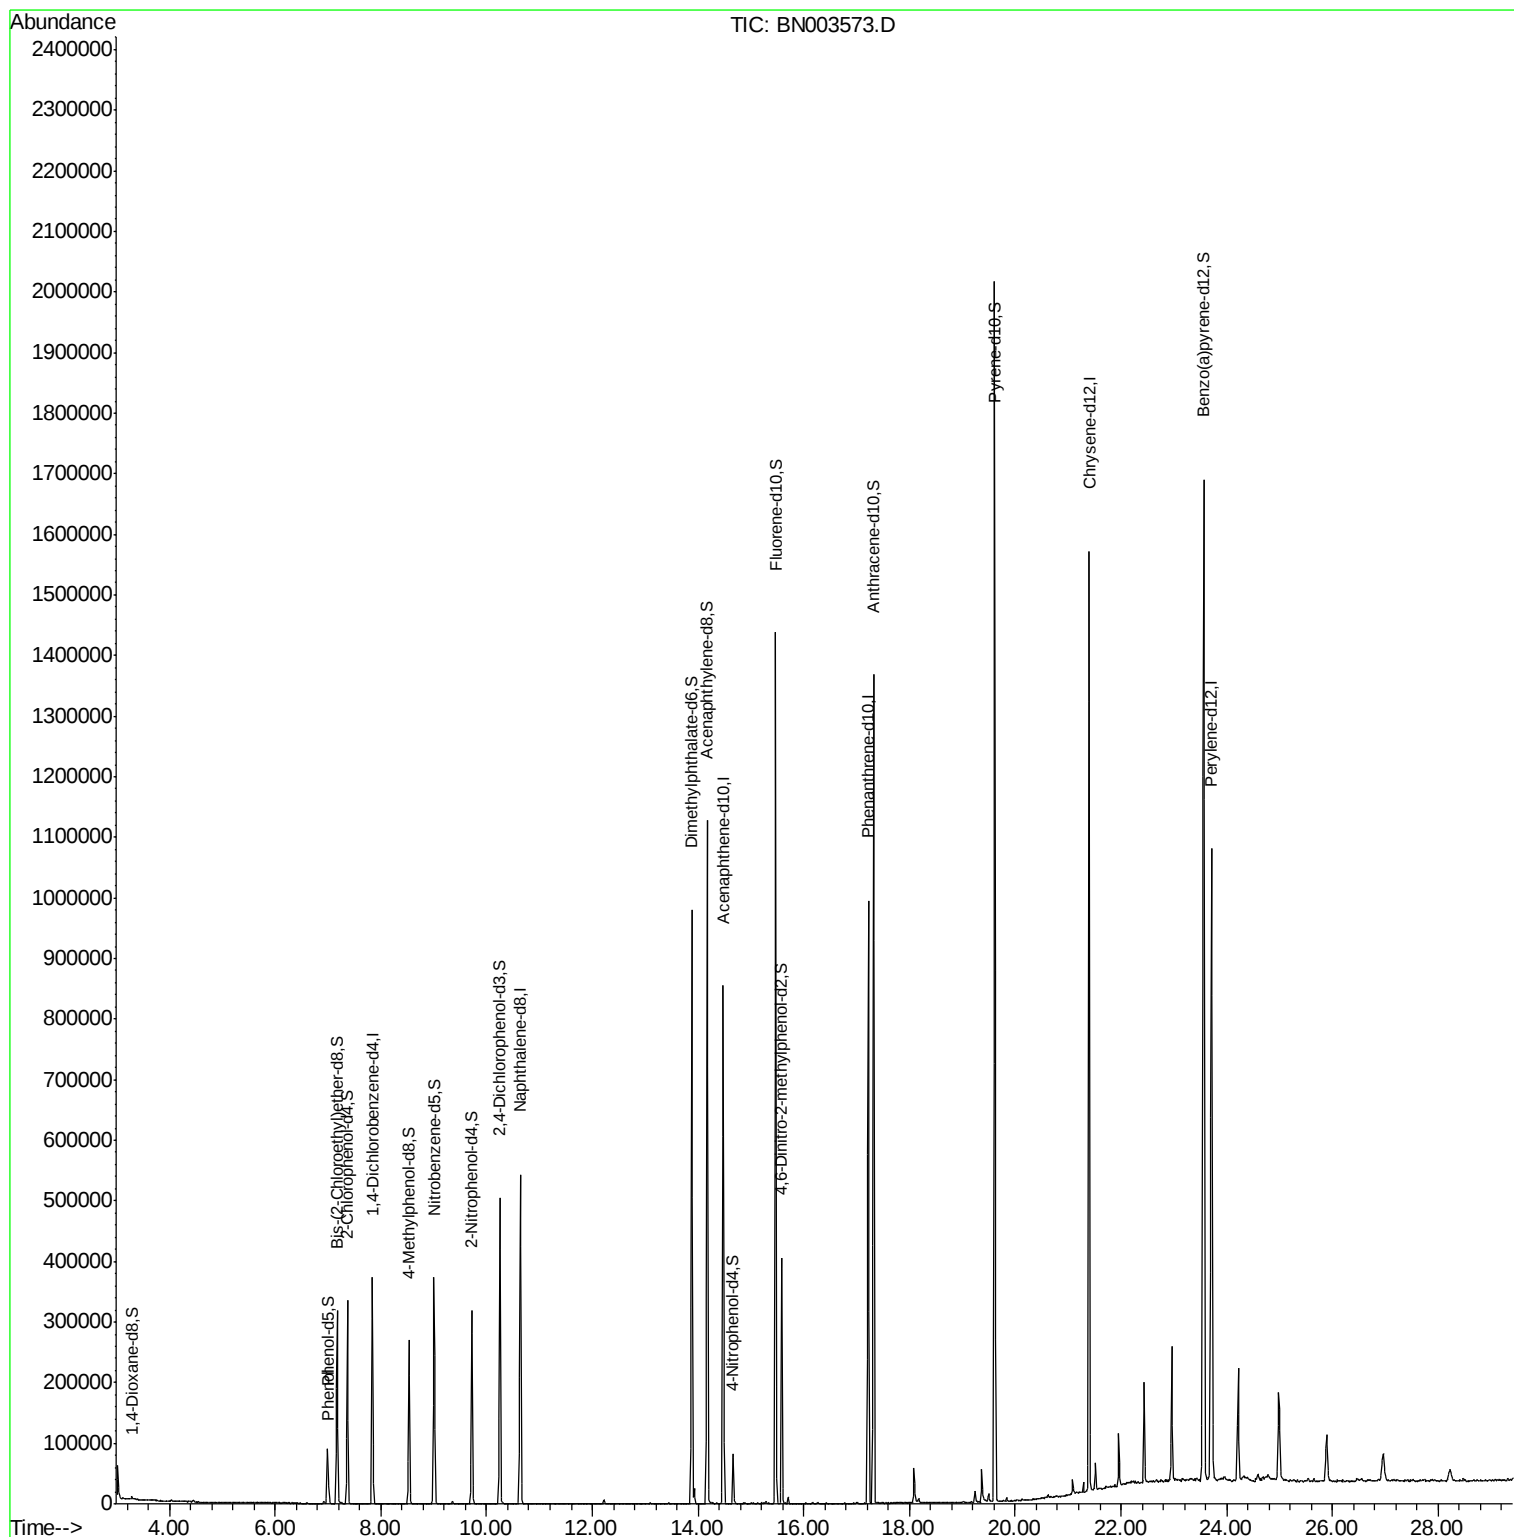

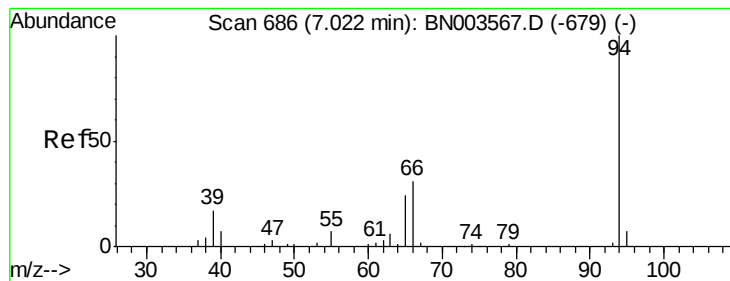

#6

Phenol

Concen: 1.748 ng/ul

RT: 7.02 min Scan# 685

Delta R.T. -0.01 min

Lab File: BN003573.D

Acq: 16 Nov 2018 20:43

Instrument :

BNA_N

ClientSampleId :

A40Z2



Tgt Ion: 94 Resp: 15238

Ion Ratio Lower Upper

94 100

65 22.9 19.2 28.8

66 35.9 25.8 38.6

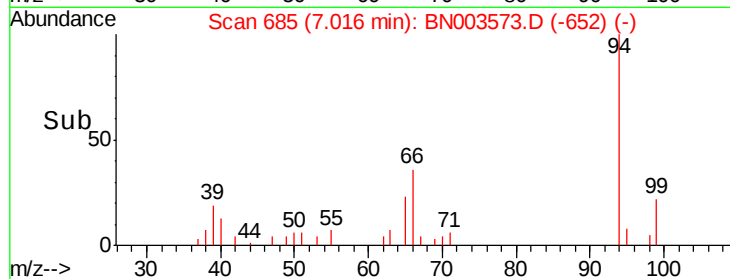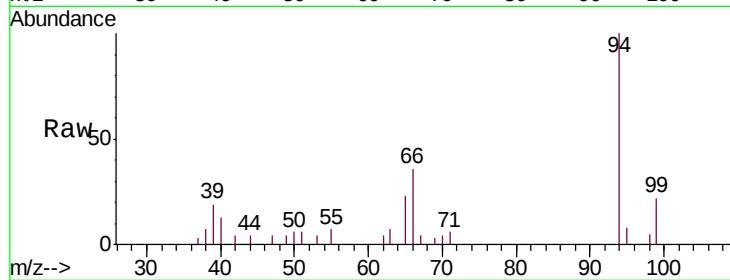

Abundance Ion 94.00 (93.70 to 94.70): BN0

Ion 65.00 (64.70 to 65.70): BN0

Ion 66.00 (65.70 to 66.70): BN0

