

Data File : BN003576.D
Acq On : 16 Nov 2018 22:29
Operator : MJ/SJ
Sample : PB114880BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK80

Quant Time: Nov 17 03:51:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	105366	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	483240	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	294129	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	679717	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	779526	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	851490	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	18703	8.39	ng/uL	0.00
5) Phenol-d5	6.99	99	371403	42.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	221729	45.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	317649	42.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	311708	42.62	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	164963	44.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	190424	45.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	322643	40.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.78	131	481695	70.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.89	166	1093313	44.84	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	1335531	44.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	198373	40.58	ng/ul	0.00
57) Fluorene-d10	15.47	176	940417	45.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	176984	37.06	ng/ul	0.00
70) Anthracene-d10	17.32	188	1469918	44.02	ng/ul	0.00
78) Pyrene-d10	19.61	212	1653815	42.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.57	264	2053207	44.54	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.53	70	6424	1.238	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003576.D
Acq On : 16 Nov 2018 22:29
Operator : MJ/SJ
Sample : PB114880BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK80

Quant Time: Nov 17 03:51:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

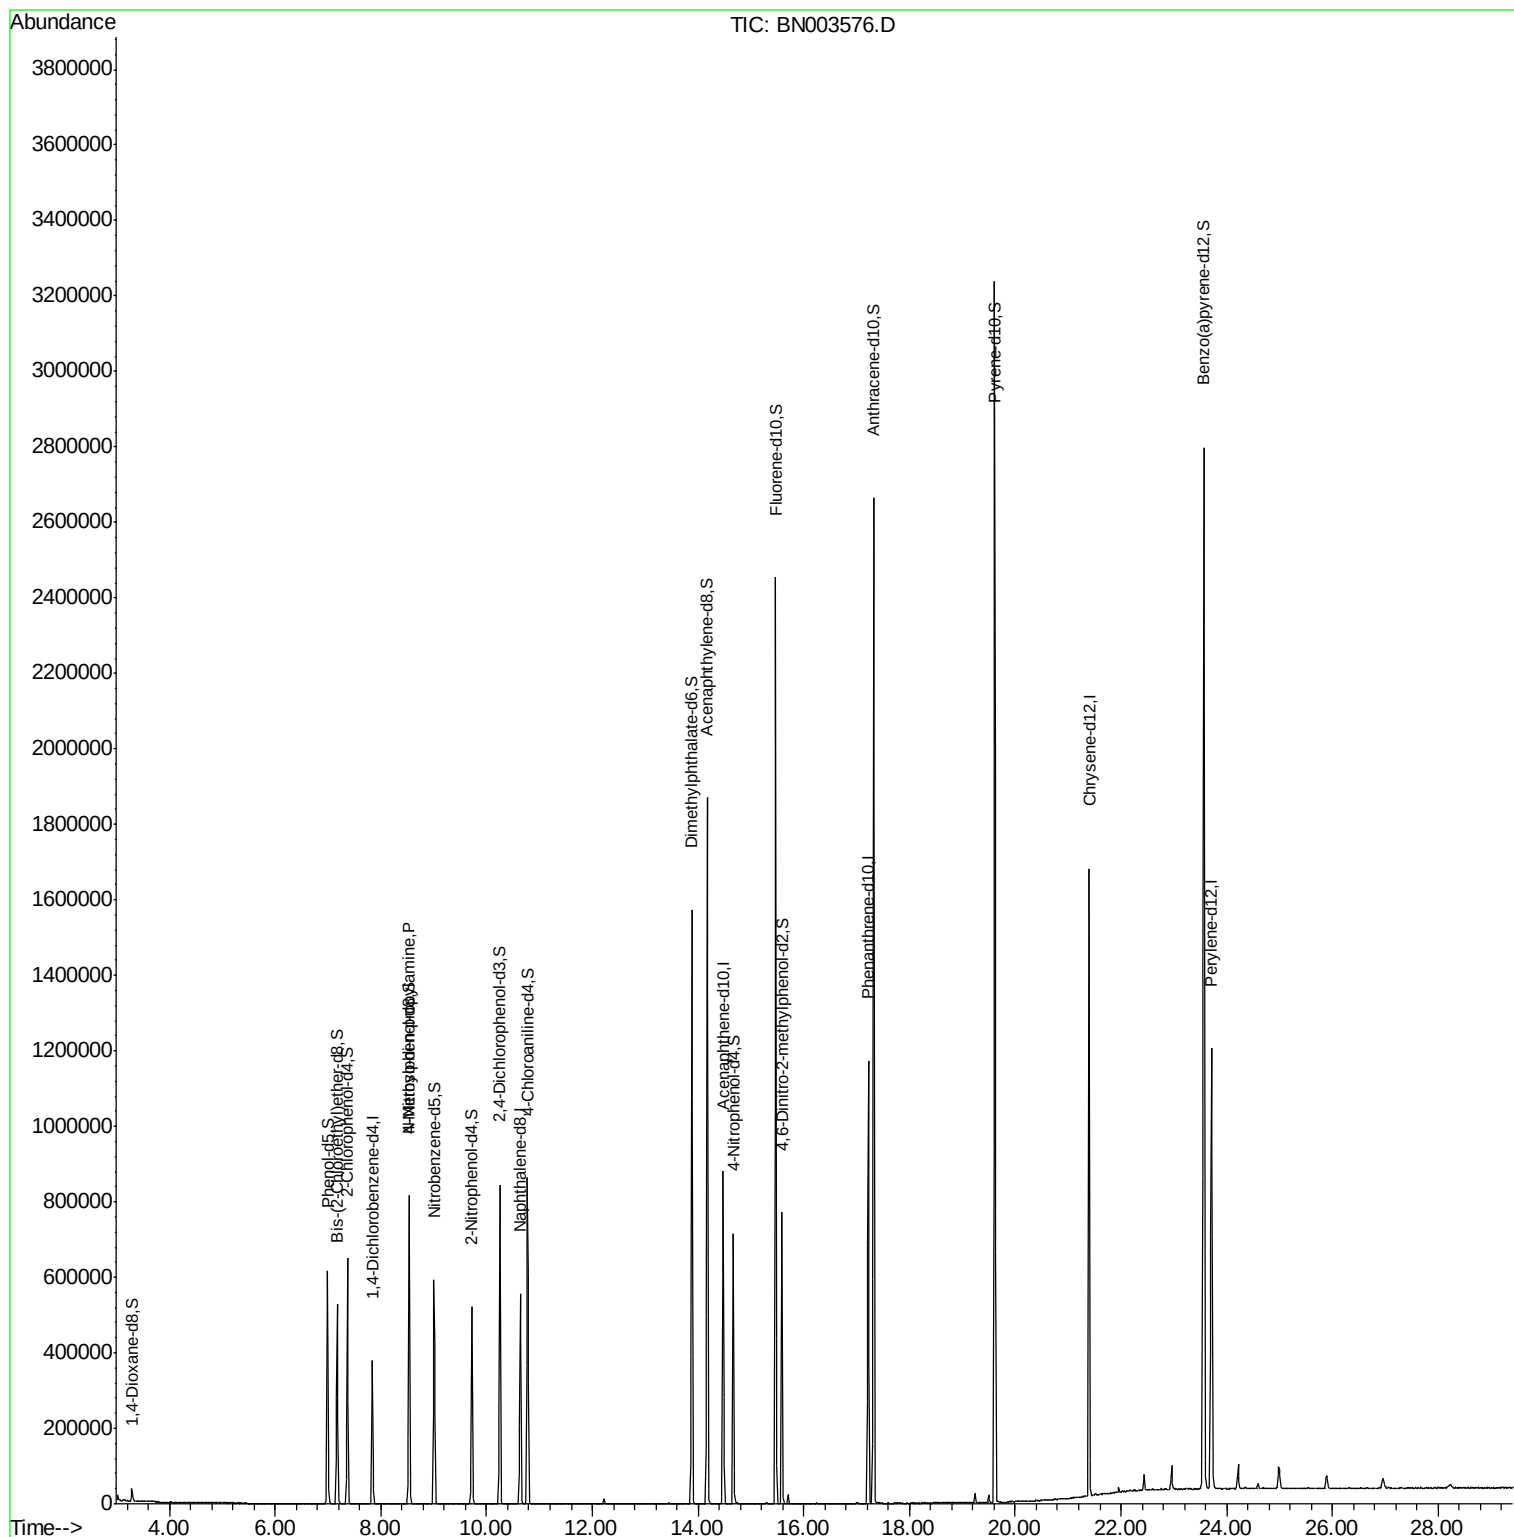

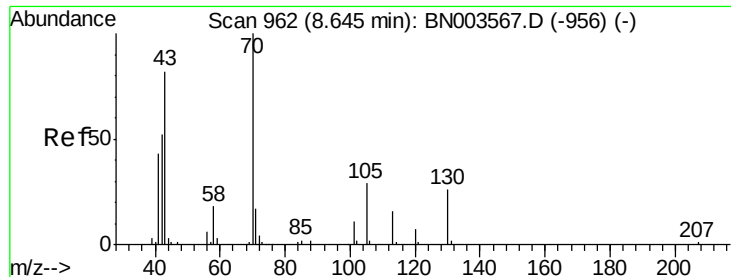

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.238 ng/ul
 RT: 8.53 min Scan# 943
 Delta R.T. -0.11 min
 Lab File: BN003576.D
 Acq: 16 Nov 2018 22:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK80

Tgt Ion:	70	Resp:	6424
Ion	Ratio	Lower	Upper
70	100		
42	374.3	41.0	61.4#
101	0.0	8.2	12.2#
130	0.0	19.8	29.6#

