

Data File : BN003578.D
Acq On : 16 Nov 2018 23:39
Operator : MJ/SJ
Sample : J5928-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y6

Quant Time: Nov 17 03:51:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	101185	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	419745	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	253591	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	623202	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	717529	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	810732	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	1136	0.53	ng/uL	0.00
5) Phenol-d5	6.99	99	26679	3.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	65182	13.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	81591	11.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	49135	7.00	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	44777	13.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	49150	13.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	87811	12.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	1086	0.18	ng/ul	0.01
43) Dimethylphthalate-d6	13.88	166	301431	14.34	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	361895	13.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	7961	1.89	ng/ul	0.00
57) Fluorene-d10	15.47	176	271214	15.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	37764	8.62	ng/ul	0.00
70) Anthracene-d10	17.32	188	436118	14.24	ng/ul	0.00
78) Pyrene-d10	19.61	212	508501	14.27	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	612473	13.95	ng/ul	-0.01


Target Compounds					Qvalue
6) Phenol	7.02	94	65228	7.752 ng/ul	98
44) Dimethylphthalate	13.93	163	184654	8.944 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003578.D
Acq On : 16 Nov 2018 23:39
Operator : MJ/SJ
Sample : J5928-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y6

Quant Time: Nov 17 03:51:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 16 22:18:27 2018
Response via : Initial Calibration

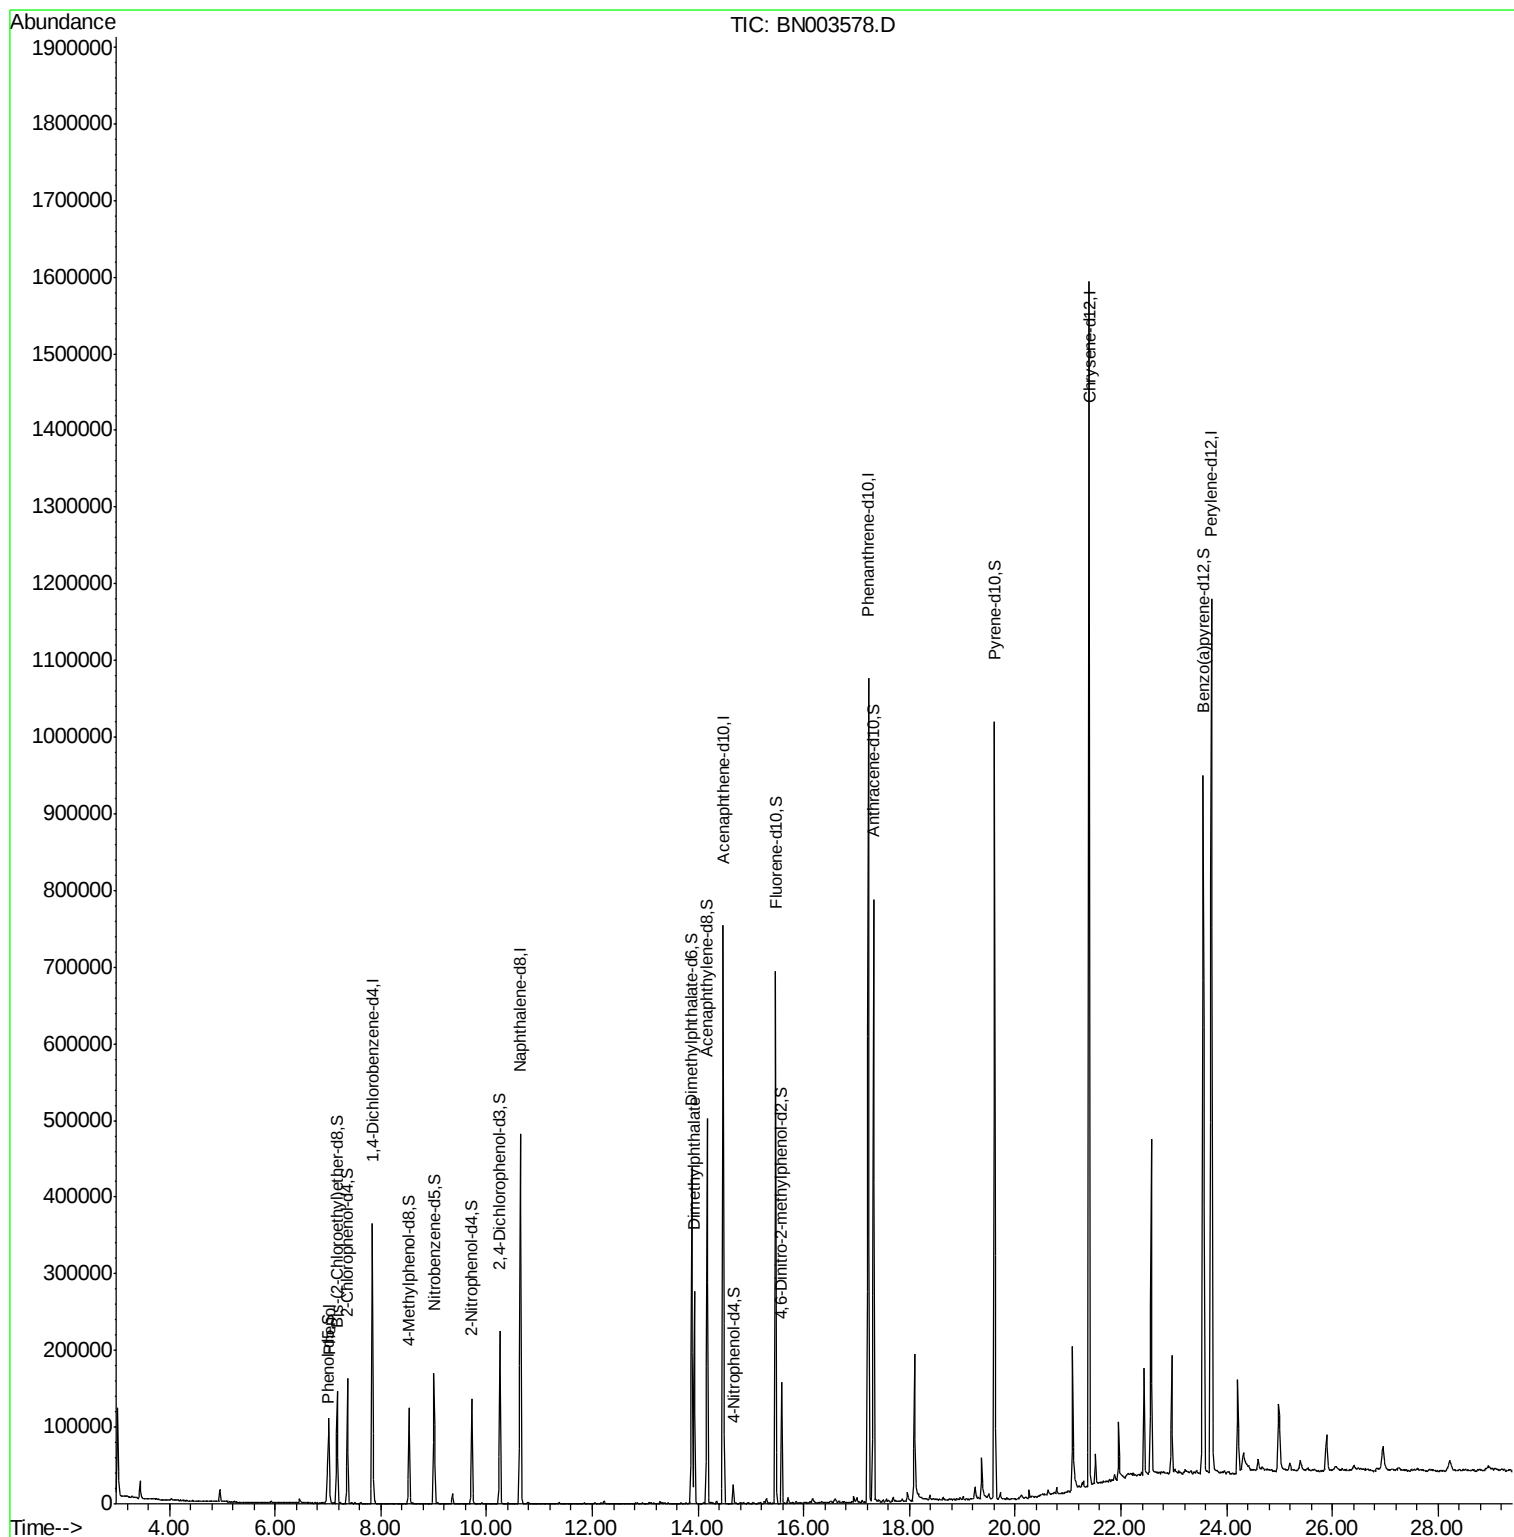

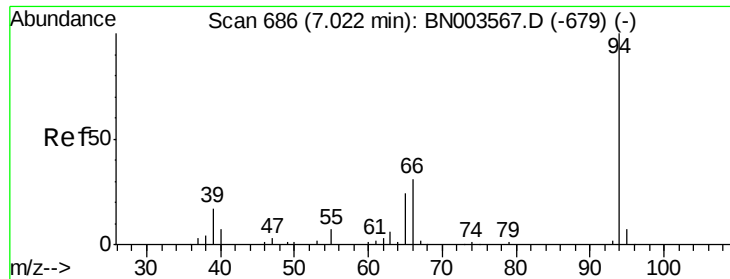

#6

Phenol

Concen: 7.752 ng/ul

RT: 7.02 min Scan# 685

Delta R.T. -0.01 min

Lab File: BN003578.D

Acq: 16 Nov 2018 23:39

Instrument :

BNA_N

ClientSampled :

A40Y6


Tgt Ion: 94 Resp: 65228

Ion Ratio Lower Upper

94 100

65 25.3 19.2 28.8




66 33.3 25.8 38.6

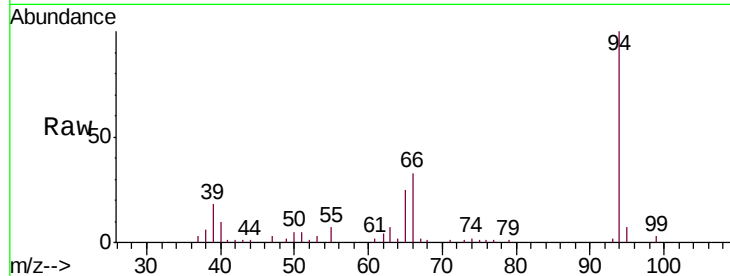

Abundance Ion 94.00 (93.70 to 94.70): BN003567.D (-679) (-)

Ion 65.00 (64.70 to 65.70): BN003567.D (-679) (-)

Ion 66.00 (65.70 to 66.70): BN003567.D (-679) (-)

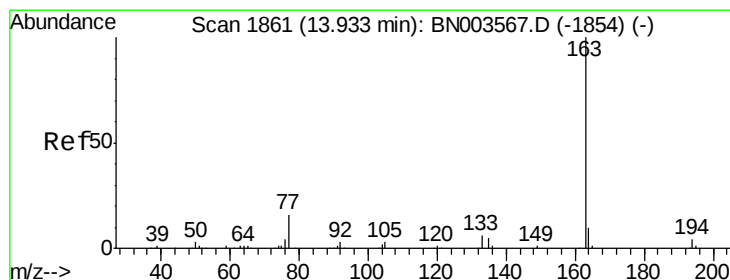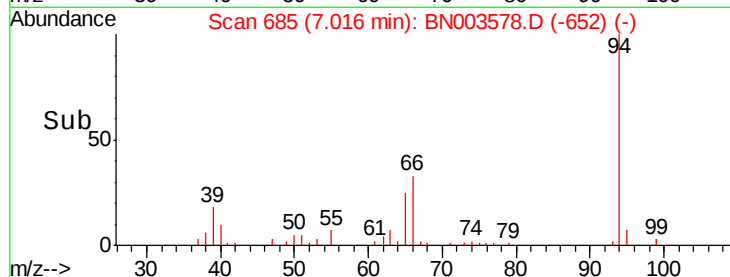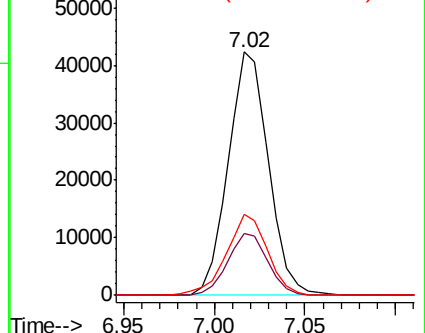

#44

Dimethylphthalate

Concen: 8.944 ng/ul

RT: 13.93 min Scan# 1860

Delta R.T. -0.01 min

Lab File: BN003578.D

Acq: 16 Nov 2018 23:39


Tgt Ion: 163 Resp: 184654

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.3 8.0 12.0

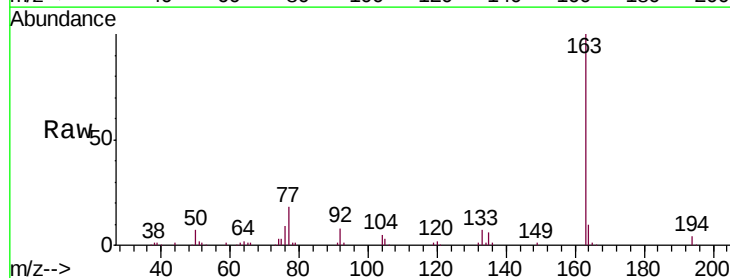

Abundance Ion 163.00 (162.70 to 163.70): BN003567.D (-1854) (-)

Ion 194.00 (193.70 to 194.70): BN003567.D (-1854) (-)

Ion 164.00 (163.70 to 164.70): BN003567.D (-1854) (-)

