

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111618\
 Data File : BN003561.D
 Acq On : 16 Nov 2018 13:06
 Operator : MJ/SJ
 Sample : J5928-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A40Z6

Quant Time: Nov 16 15:55:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 15 01:42:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	93194	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	403898	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	248026	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	569869	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	616112	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	585953	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	1943	0.99	ng/uL	0.00
5) Phenol-d5	6.99	99	40627	5.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	95723	21.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	119107	18.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	70126	10.84	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	64720	20.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	72965	20.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	123562	18.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	658	0.11	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	446620	21.72	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	530595	20.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	12655	3.07	ng/ul	0.00
57) Fluorene-d10	15.47	176	397925	23.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	63414	15.84	ng/ul	0.00
70) Anthracene-d10	17.32	188	630641	22.53	ng/ul	0.00
78) Pyrene-d10	19.61	212	716787	23.43	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	742617	23.41	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	7.02	94	35419	4.570 ng/ul	98
44) Dimethylphthalate	13.93	163	70200	3.477 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111618\
Data File : BN003561.D
Acq On : 16 Nov 2018 13:06
Operator : MJ/SJ
Sample : J5928-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z6

Quant Time: Nov 16 15:55:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 15 01:42:46 2018
Response via : Initial Calibration

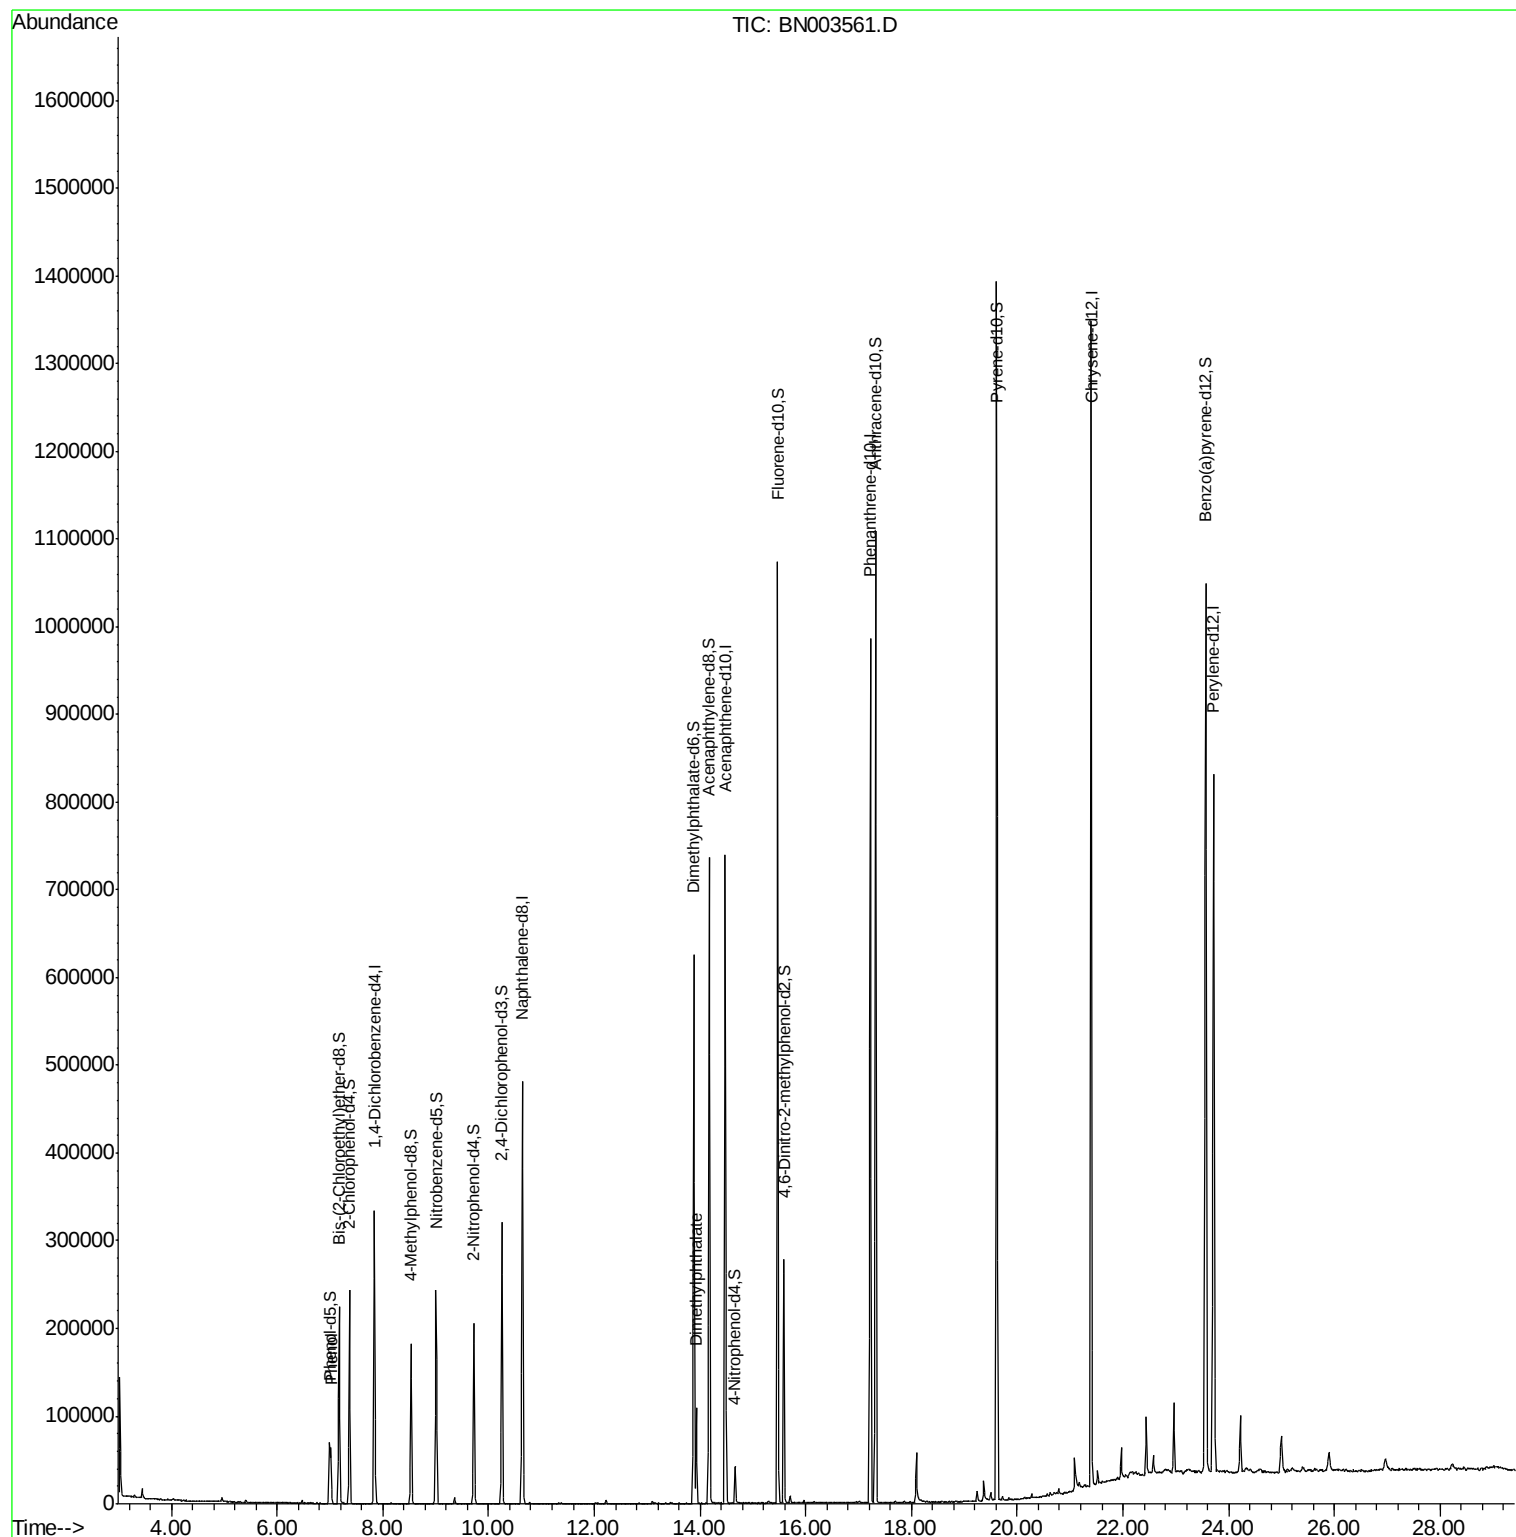

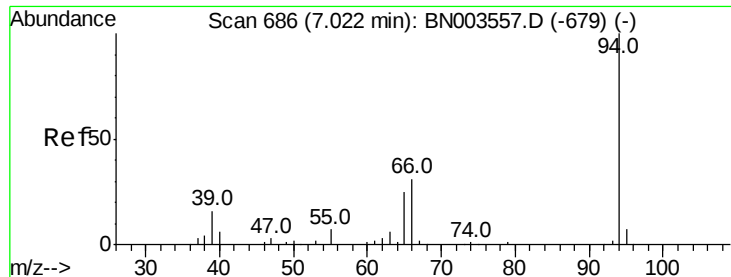

#6

Phenol

Concen: 4.570 ng/ul

RT: 7.02 min Scan# 685

Delta R.T. -0.01 min

Lab File: BN003561.D

Acq: 16 Nov 2018 13:06

Instrument :

BNA_N

ClientSampleId :

A40Z6


Tot Ion: 94 Resp: 35419

Ion Ratio Lower Upper

94 100

65 25.4 19.2 28.8




66 33.3 25.8 38.6

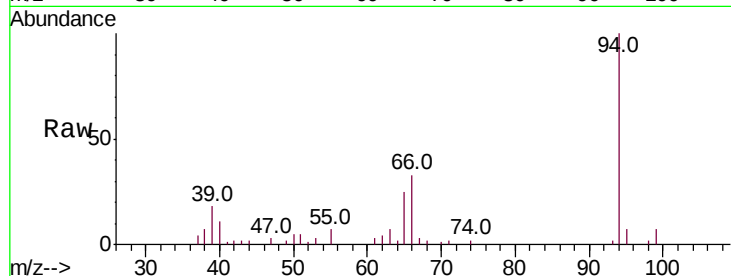

Abundance Ion 94.00 (93.70 to 94.70): BN003557.D (-679) (-)

Ion 65.00 (64.70 to 65.70): BN003557.D (-679) (-)

Ion 66.00 (65.70 to 66.70): BN003557.D (-679) (-)

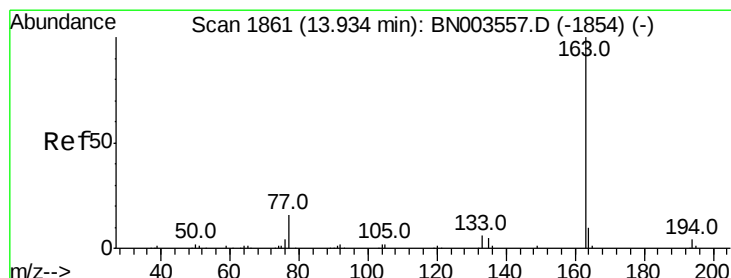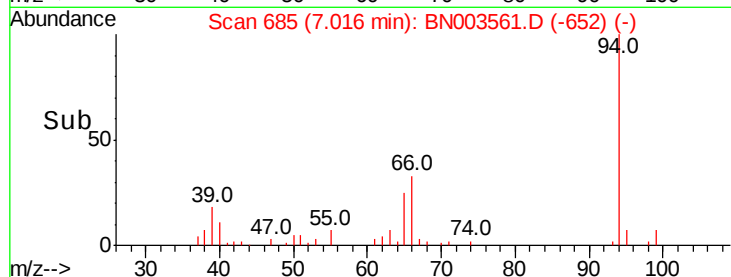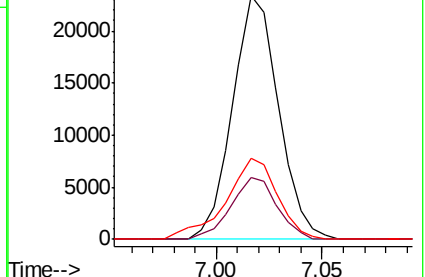

#44

Dimethylphthalate

Concen: 3.477 ng/ul

RT: 13.93 min Scan# 1860

Delta R.T. -0.01 min

Lab File: BN003561.D

Acq: 16 Nov 2018 13:06


Tgt Ion:163 Resp: 70200

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.2 8.0 12.0

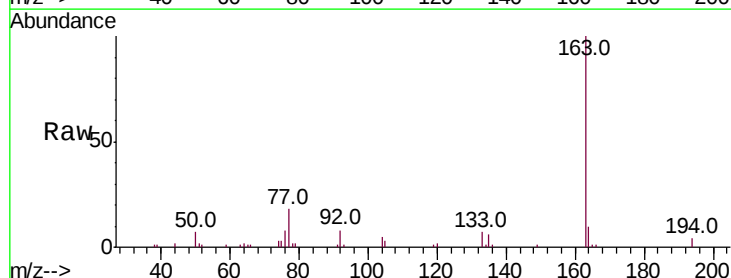

Abundance Ion 163.00 (162.70 to 163.70): BN003557.D (-1854) (-)

Ion 194.00 (193.70 to 194.70): BN003557.D (-1854) (-)

Ion 164.00 (163.70 to 164.70): BN003557.D (-1854) (-)

