


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111720\
Data File : BN012582.D
Acq On : 17 Nov 2020 11:06
Operator : CG/JU
Sample : DFTPP16
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP16

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN102220.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 18 14:31:59 2020

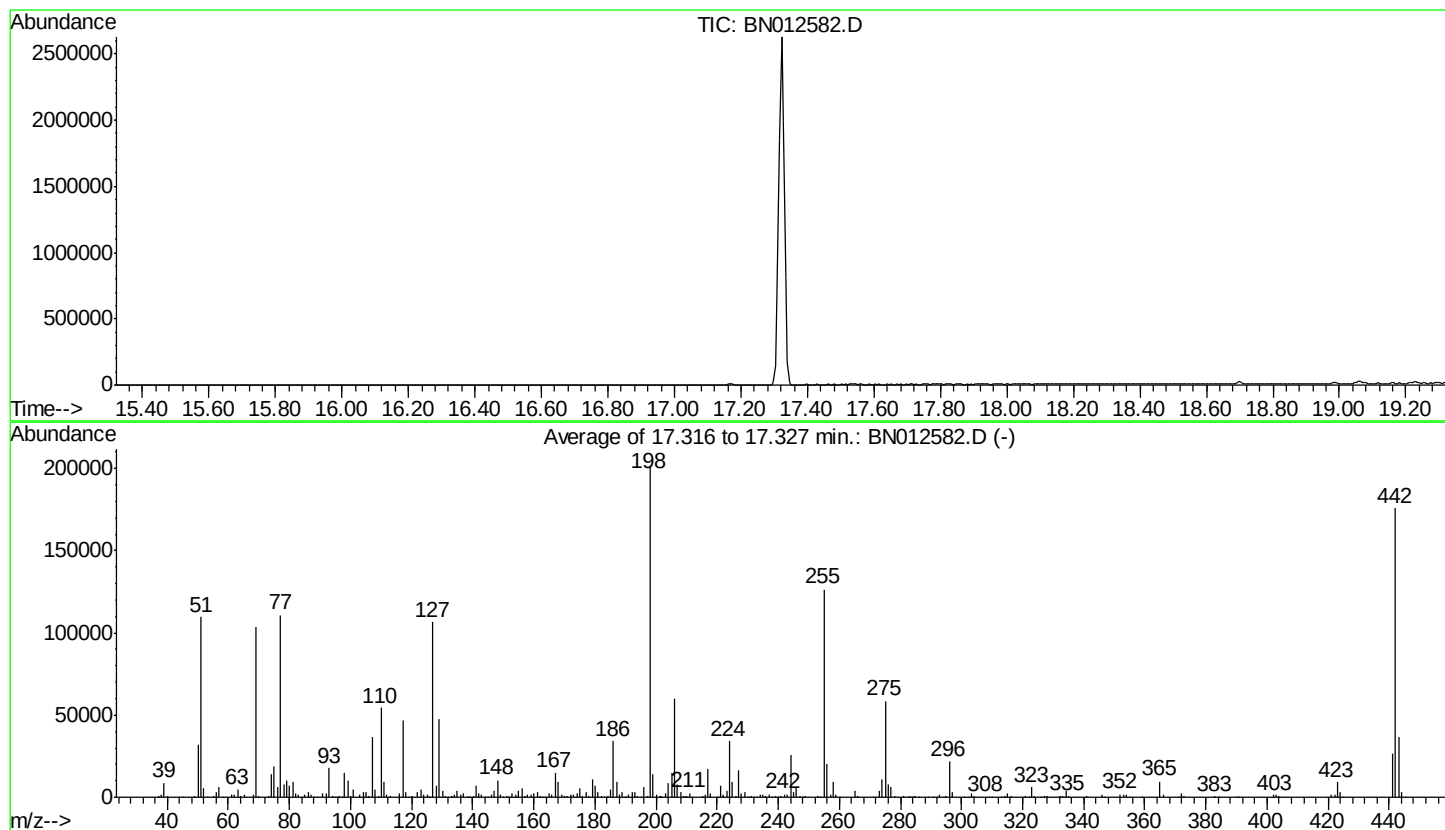

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	109768	PASS
68	69	0.00	2	1.3	1371	PASS
69	198	0.00	100	51.4	103693	PASS
70	69	0.00	2	0.6	645	PASS
127	198	10	80	52.8	106504	PASS
197	198	0.00	2	0.2	465	PASS
198	198	100	100	100.0	201792	PASS
199	198	5	9	6.8	13699	PASS
275	198	10	60	29.0	58482	PASS
365	198	1	100	4.6	9368	PASS
441	198	0.01	100	13.1	26373	PASS
442	198	50	100	87.2	175946	PASS
443	442	15	24	20.7	36450	PASS

Scan 2431 (17.286 min): BN012582.D
DFTPP16

m/z	Abundance
39.90	366.0
43.90	1005.0
48.90	463.0
73.10	410.0
192.90	341.0
207.00	1196.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

m/z	Abundance
36.90	631.0
38.10	1727.0
39.00	9304.0
39.90	1209.0
44.00	1626.0
45.10	314.0
49.00	1343.0
50.10	33264.0
51.00	110840.0
52.00	5803.0
55.10	649.0
56.00	3311.0
57.00	6033.0
61.10	1258.0
62.00	2082.0
63.00	4985.0
64.00	661.0
65.00	1534.0
68.00	1755.0
69.00	102560.0
70.00	624.0
73.10	1464.0
74.00	13085.0
75.00	18120.0
76.00	5887.0
77.00	107096.0
78.00	7822.0
79.00	10286.0
80.00	6340.0
81.00	9263.0
82.00	2217.0
83.00	1779.0
84.00	534.0
85.10	1197.0
85.90	3582.0
87.00	1278.0
87.90	412.0
91.00	1827.0
92.00	2016.0
93.00	16680.0
93.90	769.0
94.90	389.0
95.90	726.0
97.00	619.0
98.00	13917.0
99.00	10275.0
100.00	740.0
101.00	4573.0
102.90	1539.0
104.00	2901.0
104.90	3211.0
106.00	940.0
107.00	34272.0
108.00	5330.0
109.00	1017.0
110.00	50896.0
111.00	7829.0
111.90	1496.0
113.00	382.0
116.00	1893.0
117.00	41032.0
118.00	3056.0
118.90	310.0
120.10	398.0
121.90	3052.0
123.00	3973.0
124.00	1840.0
125.00	1148.0
126.10	674.0
127.00	94048.0
128.00	6627.0
129.00	44336.0
130.00	3236.0
131.10	693.0
132.00	311.0
133.00	476.0
134.00	1375.0
134.90	3776.0
136.00	1455.0
137.10	2175.0
138.00	434.0
140.00	511.0
141.00	6138.0
142.00	1984.0
142.80	1193.0
144.80	418.0
146.00	1079.0
147.00	3489.0
148.00	8912.0
149.00	1781.0
150.00	517.0
151.00	1098.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

151.90	590.0
153.00	1787.0
154.00	1473.0
155.00	2718.0
156.00	4851.0
157.00	754.0
157.80	1026.0
159.00	1465.0
160.00	1750.0
161.00	3064.0
162.20	679.0
164.00	385.0
165.00	2324.0
166.00	1924.0
167.00	13259.0
168.00	9577.0
169.00	1374.0
169.90	456.0
170.90	495.0
171.90	1386.0
173.00	1792.0
174.00	1571.0
175.10	5103.0
176.00	771.0
177.00	2391.0
178.00	985.0
179.00	8139.0
180.00	6069.0
180.90	3049.0
182.00	654.0
184.20	842.0
185.00	4589.0
186.00	29448.0
187.00	7428.0
188.00	1293.0
188.90	2554.0
191.00	1058.0
192.00	2668.0
193.00	2603.0
194.00	838.0
196.00	4573.0
198.00	170432.0
199.00	11767.0
199.90	1008.0
201.00	430.0
201.40	512.0
203.00	1821.0
204.00	8213.0
205.00	12960.0
206.00	48424.0
207.10	7161.0
207.90	2886.0
208.90	545.0
209.30	447.0
209.90	722.0
211.00	2240.0
212.10	553.0
215.00	537.0
216.10	1433.0
217.00	14980.0
218.00	1676.0
220.00	421.0
221.00	5057.0
221.80	2375.0
223.00	3093.0
224.00	25560.0
225.10	7344.0
226.10	1494.0
227.00	13325.0
227.90	2064.0
229.00	1856.0
229.90	446.0
231.10	1072.0
232.90	314.0
234.00	1311.0
235.00	1084.0
236.00	895.0
237.00	1643.0
238.00	350.0
238.90	1014.0
239.80	315.0
240.10	338.0
240.90	746.0
242.00	1571.0
243.00	1498.0
244.00	19752.0
245.10	3312.0
246.00	4990.0
246.90	1399.0
247.80	411.0
249.00	1092.0
252.90	502.0
255.00	101392.0
256.00	16199.0
256.90	1465.0
258.00	7961.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

259.00	1564.0
265.00	2903.0
265.90	452.0
273.00	2970.0
273.90	8043.0
275.00	43296.0
276.00	6534.0
277.00	4921.0
277.90	839.0
281.10	384.0
282.10	315.0
283.00	784.0
283.90	574.0
284.90	828.0
292.90	1100.0
294.00	406.0
294.90	399.0
296.00	16400.0
296.90	1670.0
303.00	1980.0
304.00	357.0
314.20	572.0
314.90	1445.0
316.00	1011.0
321.00	522.0
322.10	316.0
323.00	4531.0
324.00	639.0
327.00	963.0
327.90	604.0
332.20	316.0
333.00	453.0
334.00	2851.0
335.00	582.0
341.10	448.0
345.90	965.0
352.00	1265.0
352.90	989.0
353.90	1429.0
364.90	5907.0
366.00	1233.0
372.00	1792.0
372.90	469.0
382.90	392.0
389.90	327.0
402.00	400.0
402.90	809.0
421.10	768.0
422.00	933.0
423.00	6548.0
424.00	2799.0
425.00	413.0
441.00	19024.0
442.00	107296.0
443.00	23816.0
444.10	2315.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

m/z	Abundance
37.00	917.0
38.10	2387.0
39.00	10369.0
39.90	1064.0
43.90	1518.0
45.00	544.0
49.10	1869.0
50.00	37808.0
51.10	135296.0
52.00	6503.0
53.00	366.0
54.90	706.0
56.00	4339.0
57.00	8207.0
58.00	319.0
61.00	1594.0
62.00	1844.0
63.00	4894.0
64.00	699.0
65.10	2236.0
68.00	2358.0
69.00	128360.0
70.00	642.0
73.00	1519.0
74.10	16384.0
75.00	23936.0
76.10	7609.0
77.00	139136.0
78.10	8731.0
79.00	12039.0
79.90	9625.0
81.00	11287.0
82.00	2717.0
83.00	2109.0
84.00	333.0
85.00	1500.0
86.00	3529.0
86.90	1620.0
88.00	739.0
89.00	478.0
91.00	3203.0
92.00	3568.0
93.00	21840.0
94.00	931.0
95.00	387.0
96.10	786.0
97.00	312.0
98.00	18136.0
99.00	12124.0
100.00	1268.0
101.00	5691.0
103.00	1758.0
104.00	3983.0
105.00	4019.0
106.10	1497.0
107.00	44280.0
108.00	6034.0
109.00	1271.0
110.00	66152.0
111.00	11434.0
112.00	1730.0
112.90	561.0
116.00	2839.0
117.00	58256.0
117.90	4003.0
120.00	547.0
122.00	3265.0
123.00	5544.0
124.00	1673.0
125.00	1415.0
125.70	394.0
127.00	135744.0
128.10	9389.0
129.00	57200.0
130.00	5616.0
131.00	1405.0
131.90	484.0
132.90	659.0
134.00	1603.0
135.00	5043.0
136.10	1291.0
137.10	3146.0
137.90	407.0
139.10	311.0
140.00	868.0
141.00	7958.0
141.90	2984.0
142.80	1084.0
144.10	596.0
146.00	1801.0
147.00	4365.0
148.00	12473.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

149.00	1372.0
149.80	346.0
151.10	1297.0
152.00	417.0
153.00	2405.0
154.00	1861.0
155.00	4757.0
156.00	6569.0
157.00	974.0
157.90	1504.0
158.90	1229.0
160.00	2528.0
161.00	3885.0
161.90	1069.0
162.90	305.0
163.80	409.0
164.90	3498.0
166.10	2048.0
167.00	17728.0
168.00	10847.0
169.10	1418.0
170.00	951.0
170.80	886.0
172.00	1446.0
173.00	1746.0
174.00	2675.0
175.00	6136.0
176.00	1599.0
177.00	3581.0
177.90	1408.0
179.00	13484.0
180.00	9860.0
181.00	3405.0
182.00	552.0
184.00	962.0
185.00	6196.0
186.00	40584.0
187.00	11312.0
188.00	1624.0
189.00	3932.0
189.80	431.0
190.90	1578.0
192.00	3814.0
193.00	3885.0
194.10	632.0
194.90	455.0
196.00	7647.0
198.00	257216.0
199.00	16880.0
200.00	2064.0
201.30	933.0
201.70	666.0
202.90	2171.0
204.00	10966.0
205.00	18184.0
206.10	78960.0
207.00	11212.0
208.00	2788.0
208.90	1285.0
209.90	1349.0
210.90	3097.0
212.10	471.0
215.10	862.0
216.00	1802.0
217.00	21592.0
218.00	3041.0
221.00	8370.0
222.00	3063.0
223.00	5028.0
224.00	42016.0
225.00	12007.0
226.00	820.0
227.00	19536.0
228.00	2955.0
229.00	4481.0
230.20	621.0
231.00	1148.0
231.90	432.0
232.90	416.0
234.00	1326.0
235.10	1386.0
235.90	918.0
236.90	2355.0
238.90	1104.0
239.90	743.0
241.00	1032.0
242.00	2456.0
243.00	2556.0
244.10	31440.0
245.10	4135.0
246.00	7485.0
247.00	1264.0
248.00	443.0
249.00	1352.0
253.00	912.0
255.00	149312.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

256.00	24544.0
257.00	2418.0
258.00	10062.0
258.90	1470.0
259.90	342.0
264.90	5571.0
266.10	699.0
270.90	456.0
272.00	405.0
273.00	4710.0
274.00	12697.0
275.00	71496.0
276.00	9205.0
277.00	6987.0
278.00	1141.0
281.00	555.0
283.10	1136.0
284.10	520.0
285.00	1158.0
288.80	544.0
291.90	429.0
293.00	1295.0
293.80	305.0
294.90	882.0
296.00	26072.0
297.00	3747.0
300.90	673.0
302.00	468.0
303.00	2368.0
303.90	656.0
309.10	369.0
310.10	309.0
313.00	485.0
314.00	1460.0
314.90	2908.0
316.00	1304.0
321.10	457.0
323.00	6481.0
323.90	1528.0
325.90	412.0
326.90	1485.0
327.90	685.0
331.90	652.0
333.20	699.0
334.00	4897.0
335.10	1104.0
341.00	794.0
345.90	1540.0
346.90	409.0
352.00	1827.0
353.00	1794.0
354.00	2298.0
355.10	735.0
365.00	11645.0
366.00	1710.0
371.00	556.0
372.00	3100.0
373.00	786.0
382.90	753.0
383.90	317.0
389.80	317.0
402.00	1696.0
402.90	1831.0
404.00	946.0
421.00	2308.0
422.10	1601.0
423.00	9774.0
424.00	3769.0
425.00	305.0
441.00	30272.0
442.10	194496.0
443.00	44648.0
444.00	4132.0
445.10	344.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

m/z	Abundance
37.10	477.0
38.00	1666.0
39.10	6274.0
39.90	782.0
44.10	809.0
49.00	902.0
50.10	24368.0
51.10	83168.0
52.00	3872.0
55.00	543.0
56.10	2836.0
57.00	4776.0
60.90	1116.0
62.00	1187.0
63.00	3722.0
64.00	384.0
65.00	1448.0
69.00	80160.0
70.00	669.0
73.10	880.0
74.00	12689.0
75.00	13446.0
76.10	4910.0
77.10	86832.0
78.10	5865.0
79.00	7586.0
80.00	5532.0
81.00	7346.0
82.00	1317.0
83.00	1206.0
85.00	1023.0
86.10	2241.0
87.00	844.0
87.70	494.0
91.00	1636.0
92.00	1727.0
93.00	14729.0
93.90	980.0
96.10	866.0
98.00	12569.0
99.00	8233.0
100.00	648.0
101.00	3467.0
103.00	1230.0
104.00	2741.0
104.90	2206.0
106.10	659.0
107.00	31776.0
108.00	3341.0
109.10	1173.0
110.00	46488.0
111.00	8030.0
112.00	1125.0
112.90	526.0
116.00	2138.0
117.00	39856.0
118.00	2952.0
119.00	427.0
120.00	308.0
122.00	2168.0
123.00	3645.0
124.00	1584.0
124.90	1203.0
127.00	89720.0
128.00	6191.0
129.00	40544.0
130.00	3796.0
130.90	825.0
132.90	357.0
134.00	1527.0
135.00	3320.0
136.00	1361.0
137.00	2243.0
138.70	344.0
140.10	766.0
141.00	6141.0
142.00	1751.0
142.90	1617.0
144.00	639.0
146.00	1309.0
147.00	3846.0
148.00	9891.0
149.00	1810.0
150.90	723.0
151.60	682.0
153.00	2062.0
154.00	1331.0
155.00	3454.0
156.10	4101.0
157.20	928.0
157.90	1176.0
158.90	931.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

160.10	1738.0
161.00	2726.0
161.90	693.0
165.00	2251.0
165.90	1529.0
167.00	14030.0
168.00	7276.0
168.90	1124.0
170.00	461.0
170.80	517.0
172.00	1245.0
173.00	1482.0
174.00	2744.0
175.00	4239.0
176.00	1099.0
176.90	2375.0
178.10	425.0
179.00	10243.0
180.00	6082.0
181.00	2211.0
182.00	556.0
183.00	430.0
183.80	672.0
185.00	4272.0
186.00	31728.0
187.00	8355.0
188.10	1574.0
189.00	2205.0
190.10	467.0
191.00	1208.0
192.00	3001.0
193.10	3817.0
194.00	446.0
195.00	351.0
196.00	5767.0
197.10	1397.0
198.00	177728.0
199.00	12450.0
200.00	1046.0
201.50	772.0
202.90	1936.0
204.10	6865.0
205.00	12575.0
206.00	52384.0
207.00	8014.0
208.00	2849.0
209.00	1067.0
210.10	870.0
211.00	2207.0
215.00	918.0
216.00	1589.0
217.00	15502.0
217.90	1798.0
219.90	406.0
220.30	695.0
221.00	7284.0
222.00	2512.0
223.00	3396.0
224.00	34416.0
225.10	8072.0
226.00	1057.0
227.00	17080.0
228.10	1815.0
229.00	3075.0
229.90	455.0
231.00	1190.0
231.90	374.0
233.90	1065.0
234.90	1486.0
236.00	797.0
237.10	1490.0
239.00	817.0
240.00	796.0
241.00	1149.0
242.00	1743.0
244.00	25056.0
245.00	3116.0
246.00	5642.0
247.00	909.0
248.90	891.0
253.10	517.0
253.90	1017.0
255.00	128152.0
256.00	19304.0
257.00	1607.0
257.90	10268.0
259.00	1238.0
260.00	454.0
264.90	3560.0
266.10	582.0
270.90	635.0
272.00	335.0
273.00	4190.0
274.00	11931.0
275.00	60656.0
276.00	8036.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16

276.90	6863.0
277.90	1497.0
281.00	631.0
283.00	510.0
285.10	957.0
286.00	315.0
290.80	348.0
292.00	302.0
292.90	1218.0
294.00	489.0
294.90	654.0
296.00	22792.0
297.00	3054.0
302.00	536.0
303.10	2171.0
304.00	675.0
308.00	412.0
312.90	462.0
314.00	1171.0
315.00	2530.0
316.10	952.0
320.90	578.0
323.10	6648.0
324.00	1170.0
327.00	1136.0
328.00	663.0
332.00	621.0
333.00	806.0
334.10	4216.0
335.00	1076.0
341.00	1200.0
346.00	1967.0
346.90	428.0
351.90	2039.0
353.00	1241.0
354.00	2036.0
355.00	402.0
358.90	347.0
365.00	10552.0
365.90	1253.0
370.90	591.0
372.00	3278.0
372.90	533.0
382.90	833.0
384.10	376.0
390.90	467.0
402.00	1657.0
403.00	1535.0
404.00	522.0
420.90	1102.0
422.00	1742.0
423.00	11627.0
424.00	3895.0
424.80	457.0
441.00	29824.0
442.00	226048.0
443.00	40888.0
444.00	3721.0

Instrument :
BNA_N
ClientSampleId :
DFTPP16