
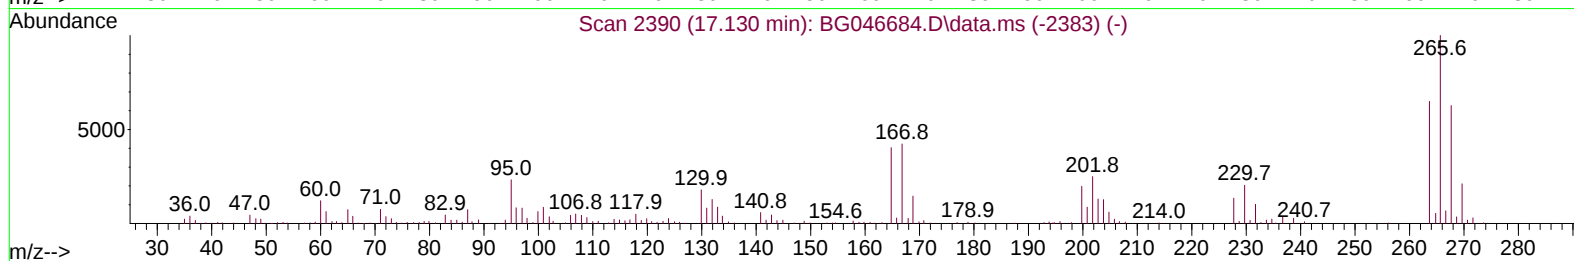
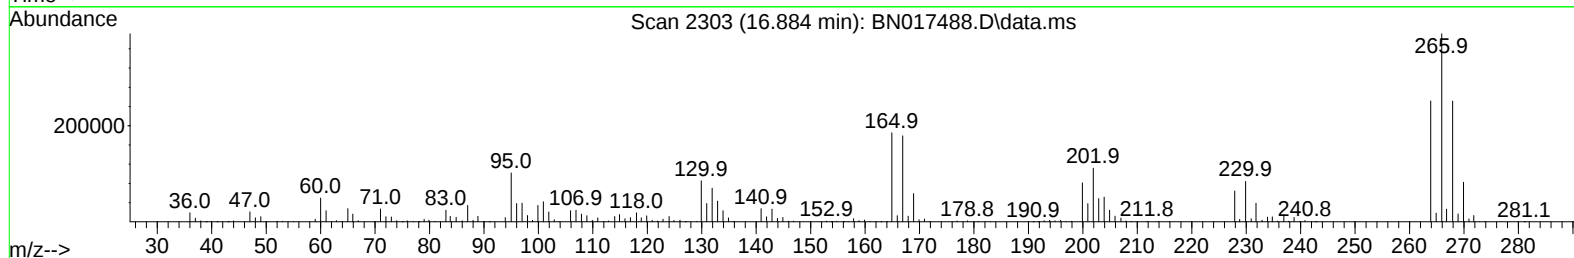


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111721\
Data File : BN017488.D
Acq On : 17 Nov 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:14:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 17 10:14:41 2021
Response via : Initial Calibration

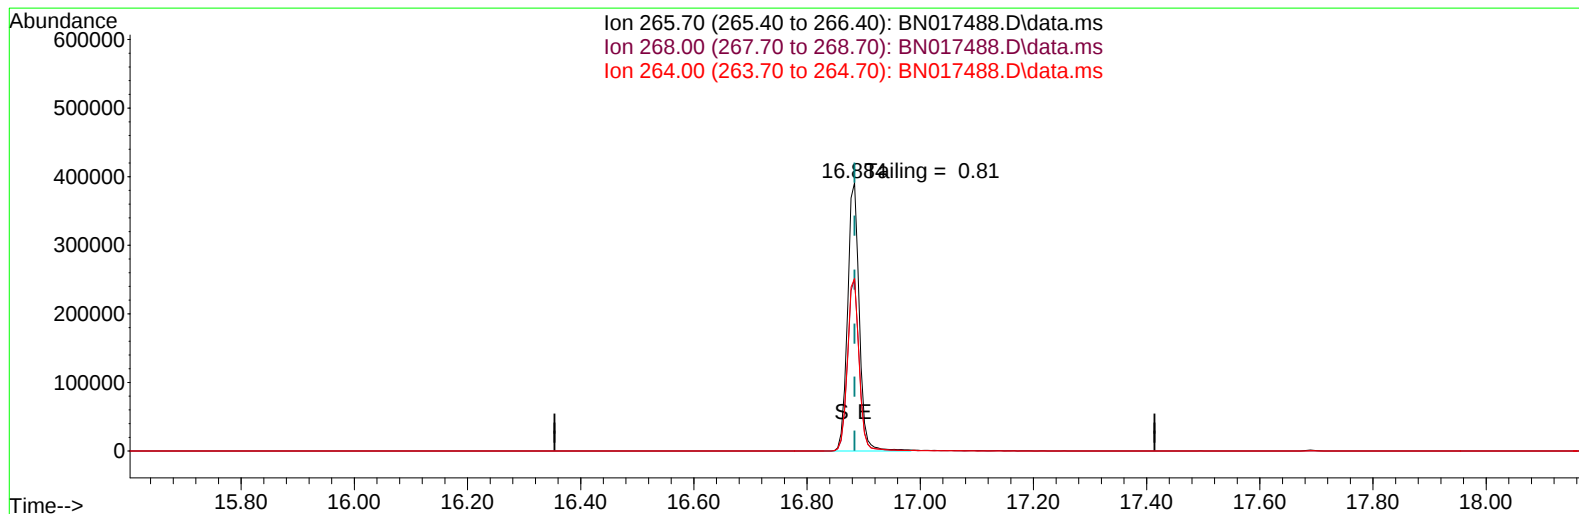

TIC: BN017488.D\data.ms

(70) Pentachlorophenol (C)




16.884min (0.000) 20344.75 ng

response 564240

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	64.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111721\
Data File : BN017488.D
Acq On : 17 Nov 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:14:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 17 10:14:41 2021
Response via : Initial Calibration

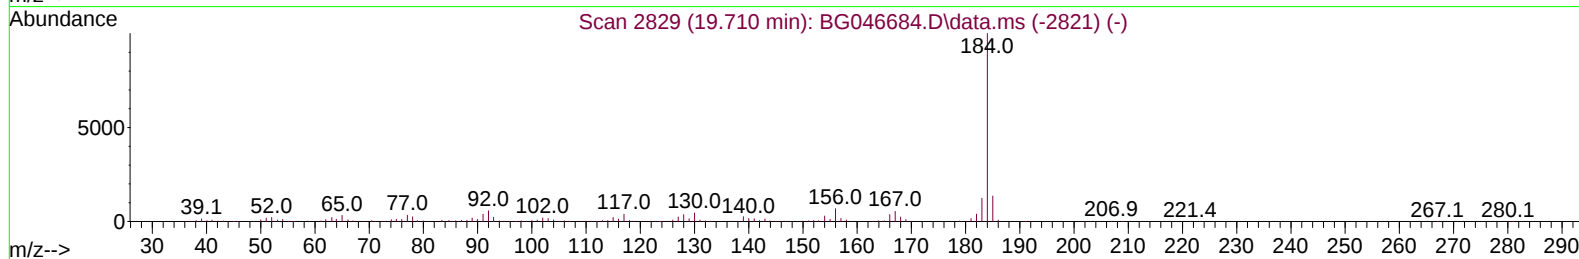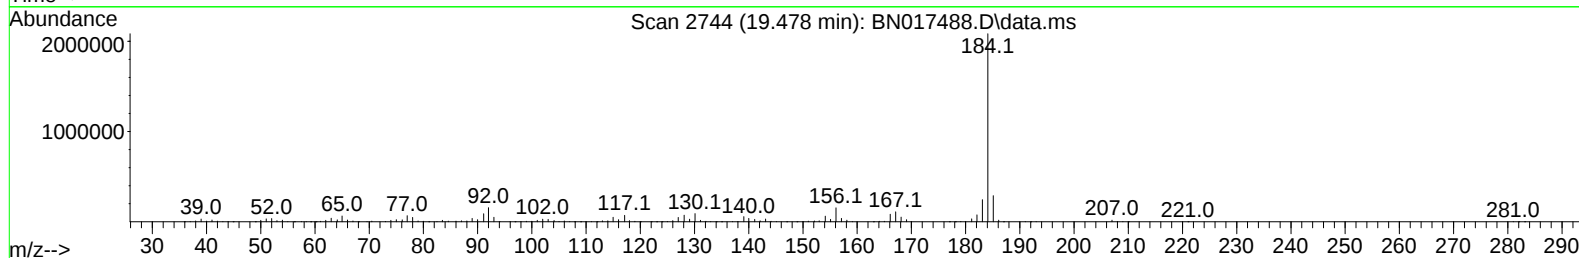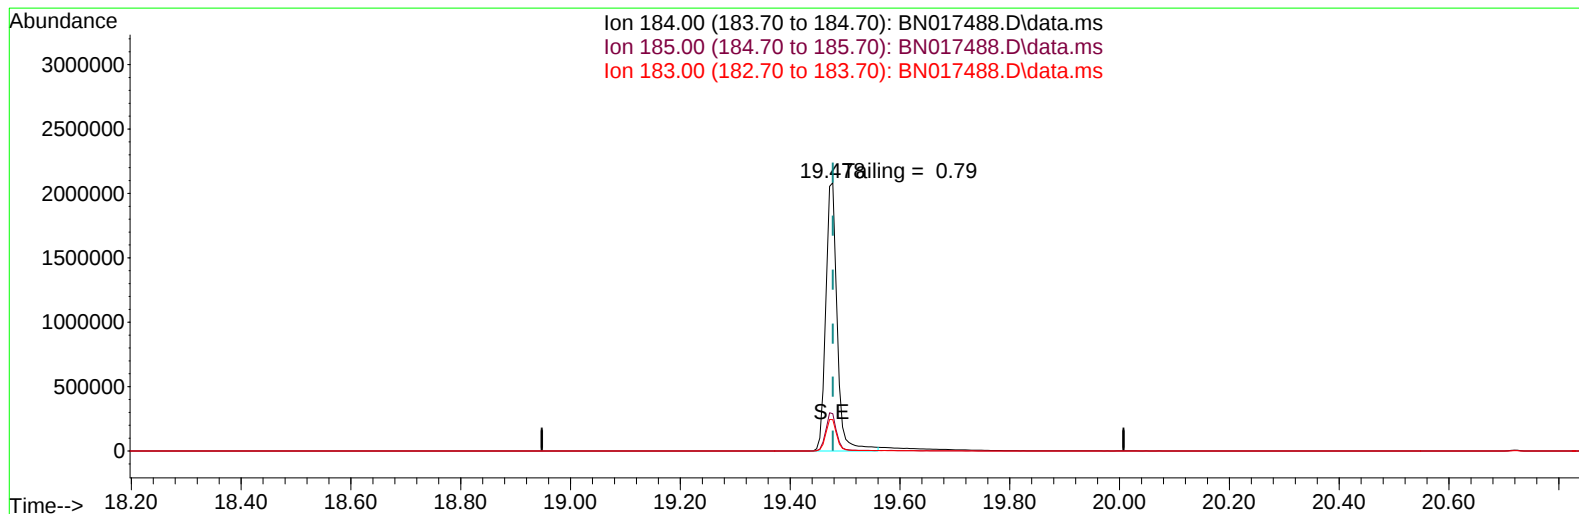

TIC: BN017488.D\data.ms

(77) Benzidine

19.478min (0.000) 0.00 ng

response 3198001

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	11.72
0.00	0.00	0.00