
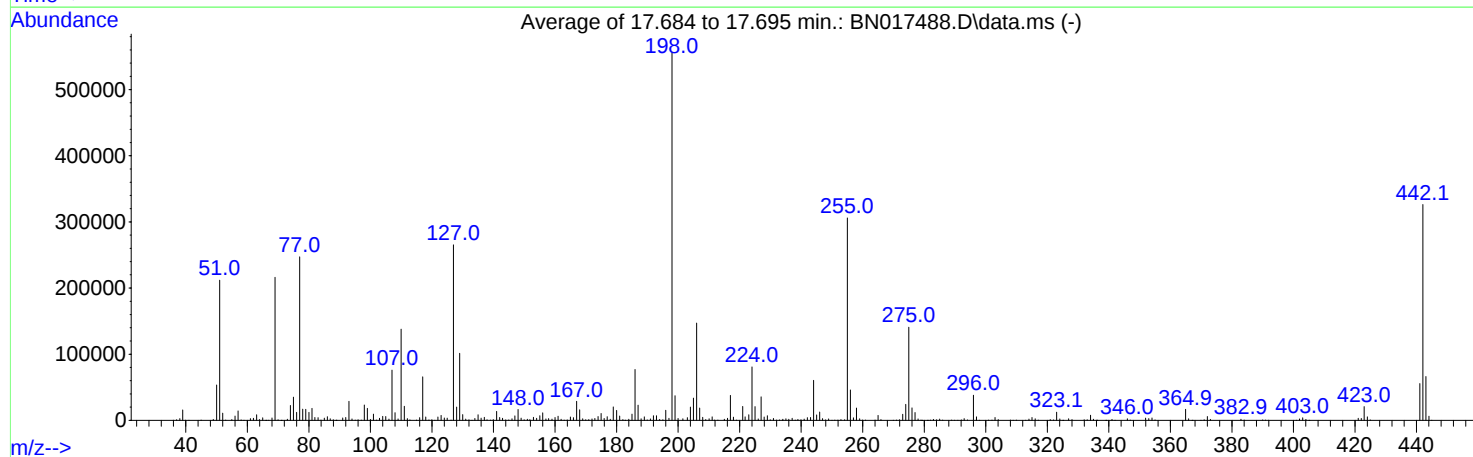


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111721\
 Data File : BN017488.D
 Acq On : 17 Nov 2021 08:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN111621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 16 14:06:59 2021

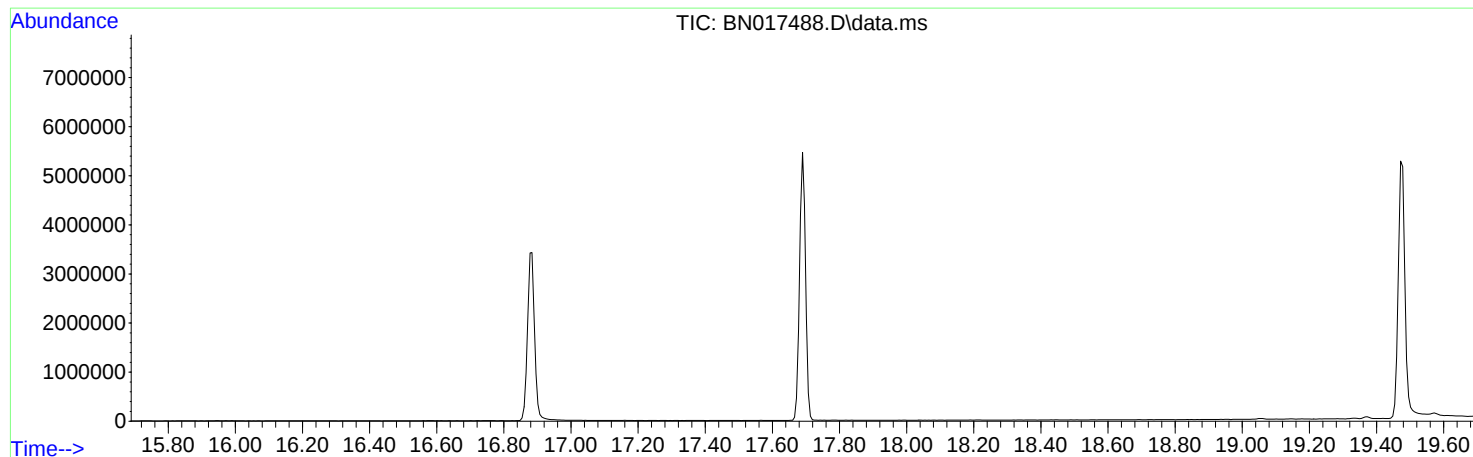




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	211947	PASS
68	69	0.00	2	1.7	3689	PASS
69	198	0.00	100	38.9	216171	PASS
70	69	0.00	2	0.5	1082	PASS
127	198	10	80	47.7	265280	PASS
197	198	0.00	2	0.6	3148	PASS
198	198	100	100	100.0	556075	PASS
199	198	5	9	6.7	37173	PASS
275	198	10	60	25.3	140779	PASS
365	198	1	100	3.0	16587	PASS
441	198	0.01	100	10.0	55611	PASS
442	442	50	100	100.0	326379	PASS
443	442	15	24	20.3	66368	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111721\
 Data File : BN017488.D
 Acq On : 17 Nov 2021 08:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 17 10:14:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 17 10:14:41 2021
 Response via : Initial Calibration

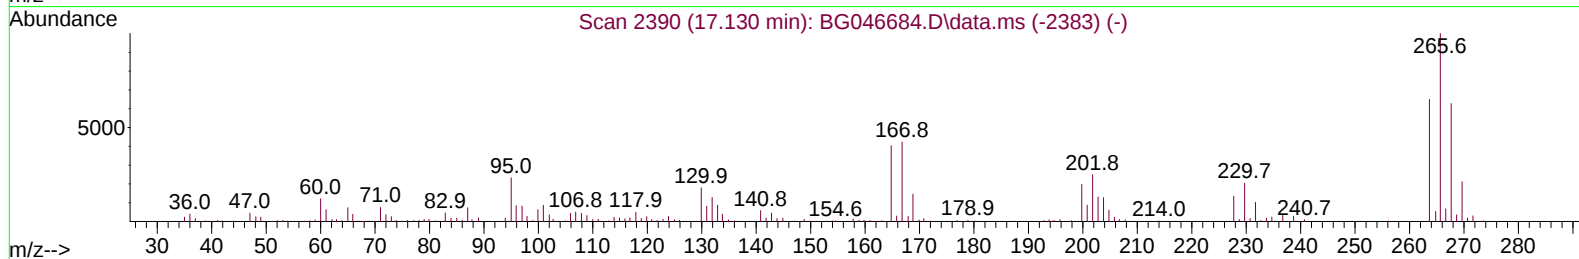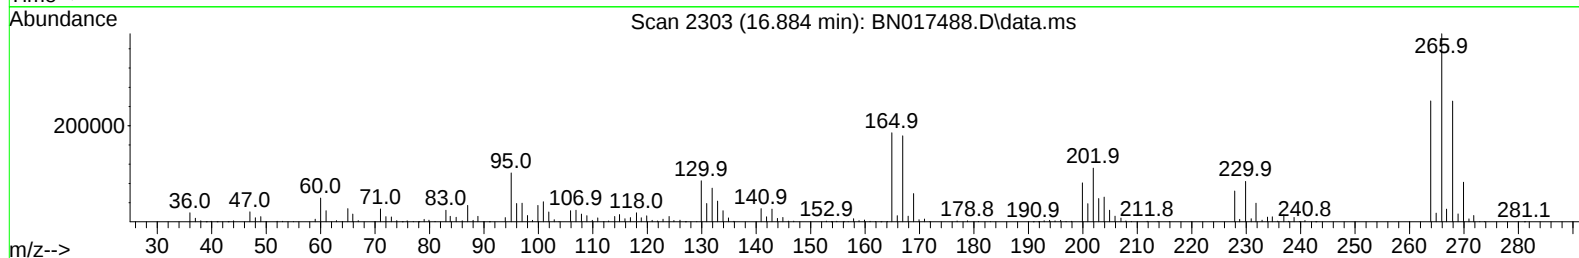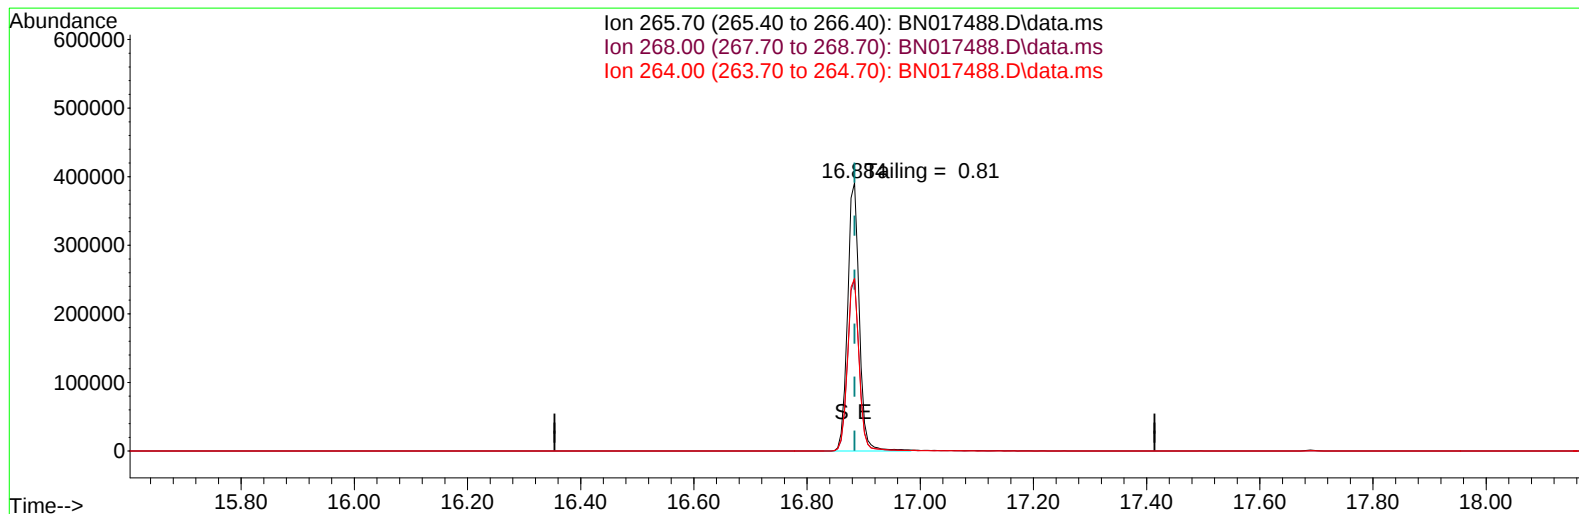

TIC: BN017488.D\data.ms

(70) Pentachlorophenol (C)

16.884min (0.000) 20344.75 ng




response 564240

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	64.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111721\
Data File : BN017488.D
Acq On : 17 Nov 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 17 10:14:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 17 10:14:41 2021
Response via : Initial Calibration

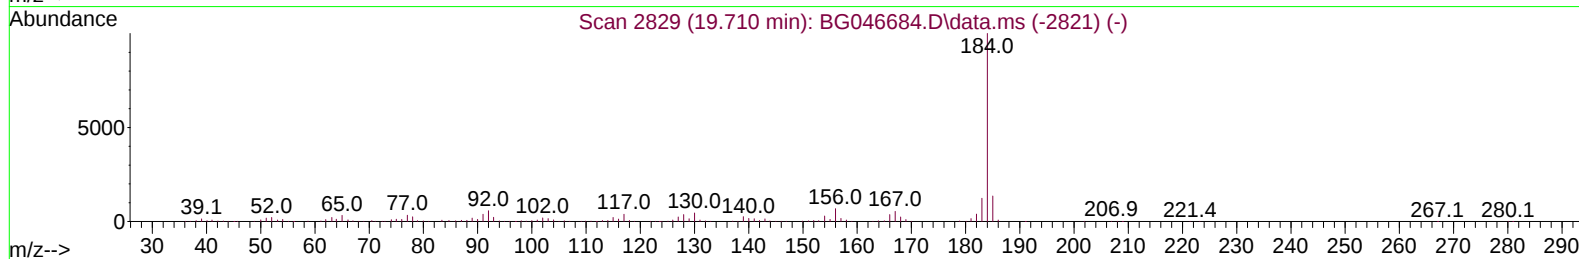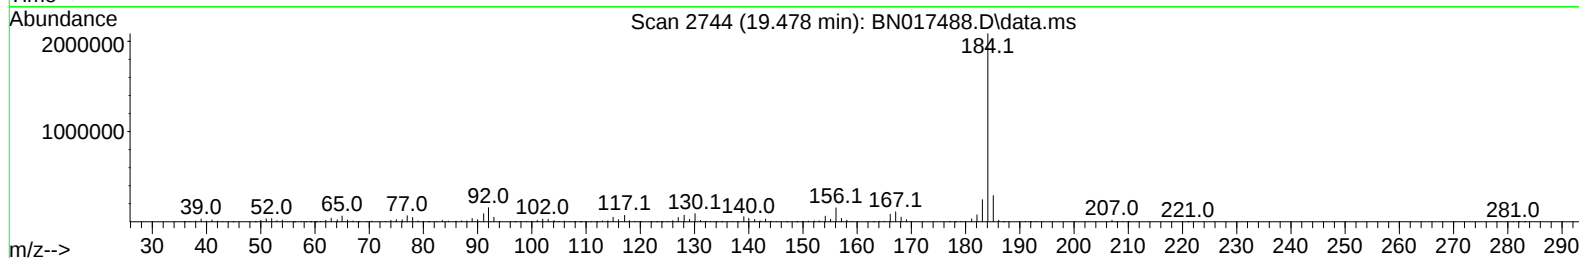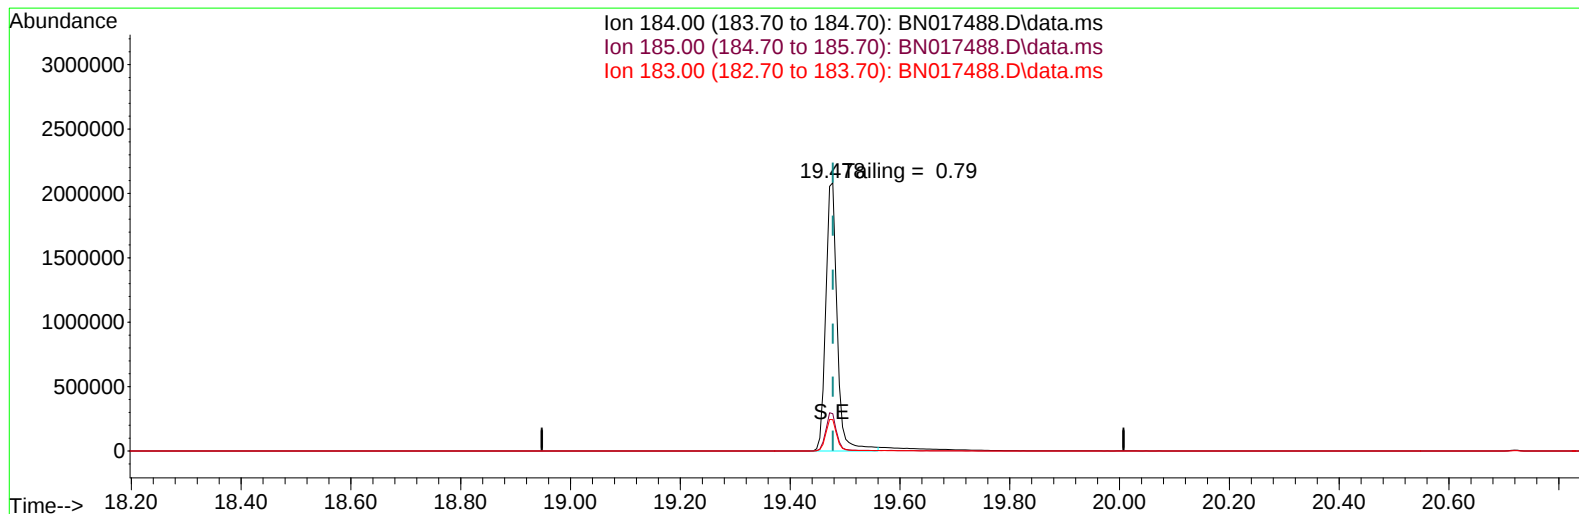

TIC: BN017488.D\data.ms

(77) Benzidine

19.478min (0.000) 0.00 ng

response 3198001

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2021	BNA_N	<u>BN017488.D</u>
Compound Name	Response	Retention Time
DDT	1739416	20.71
DDD	48061	20.27
DDE	19111	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67172	1806588	3.72

Instrument :
BNA_N
ClientSampleId :
DFTPP