

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022725.D
 Acq On : 17 Nov 2022 18:19
 Operator : CG/JU
 Sample : PB149134BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK134

Quant Time: Nov 17 22:12:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	16313	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	79471	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	55695	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	121481	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	127517	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264	133140	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	8172	17.103	ng/uL	0.00
4) Pyridine-d5	3.623	84	69747	51.617	ng/ul	0.00
7) Phenol-d5	7.028	99	129707	84.186	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	88897	96.232	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	97694	86.582	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	109173	89.755	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	52779	85.800	ng/ul	0.00
24) 2-Nitrophenol-d4	9.758	143	58984	85.936	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	94029	80.358	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	193499	108.564	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	385017	95.042	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	387671	86.852	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	68959	85.390	ng/ul	0.00
60) Fluorene-d10	15.522	176	312126	93.943	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	56536	73.218	ng/ul	0.00
73) Anthracene-d10	17.381	188	508855	95.660	ng/ul	0.00
81) Pyrene-d10	19.686	212	591075	89.444	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	661796	98.882	ng/ul	0.00
Target Compounds						Qvalue
17) N-Nitroso-di-n-propyla...	8.587	70	3018	2.917	ng/ul#	1
23) Isophorone	9.758	82	6079	1.907	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022725.D
Acq On : 17 Nov 2022 18:19
Operator : CG/JU
Sample : PB149134BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK134

Quant Time: Nov 17 22:12:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 17 22:08:43 2022
Response via : Initial Calibration




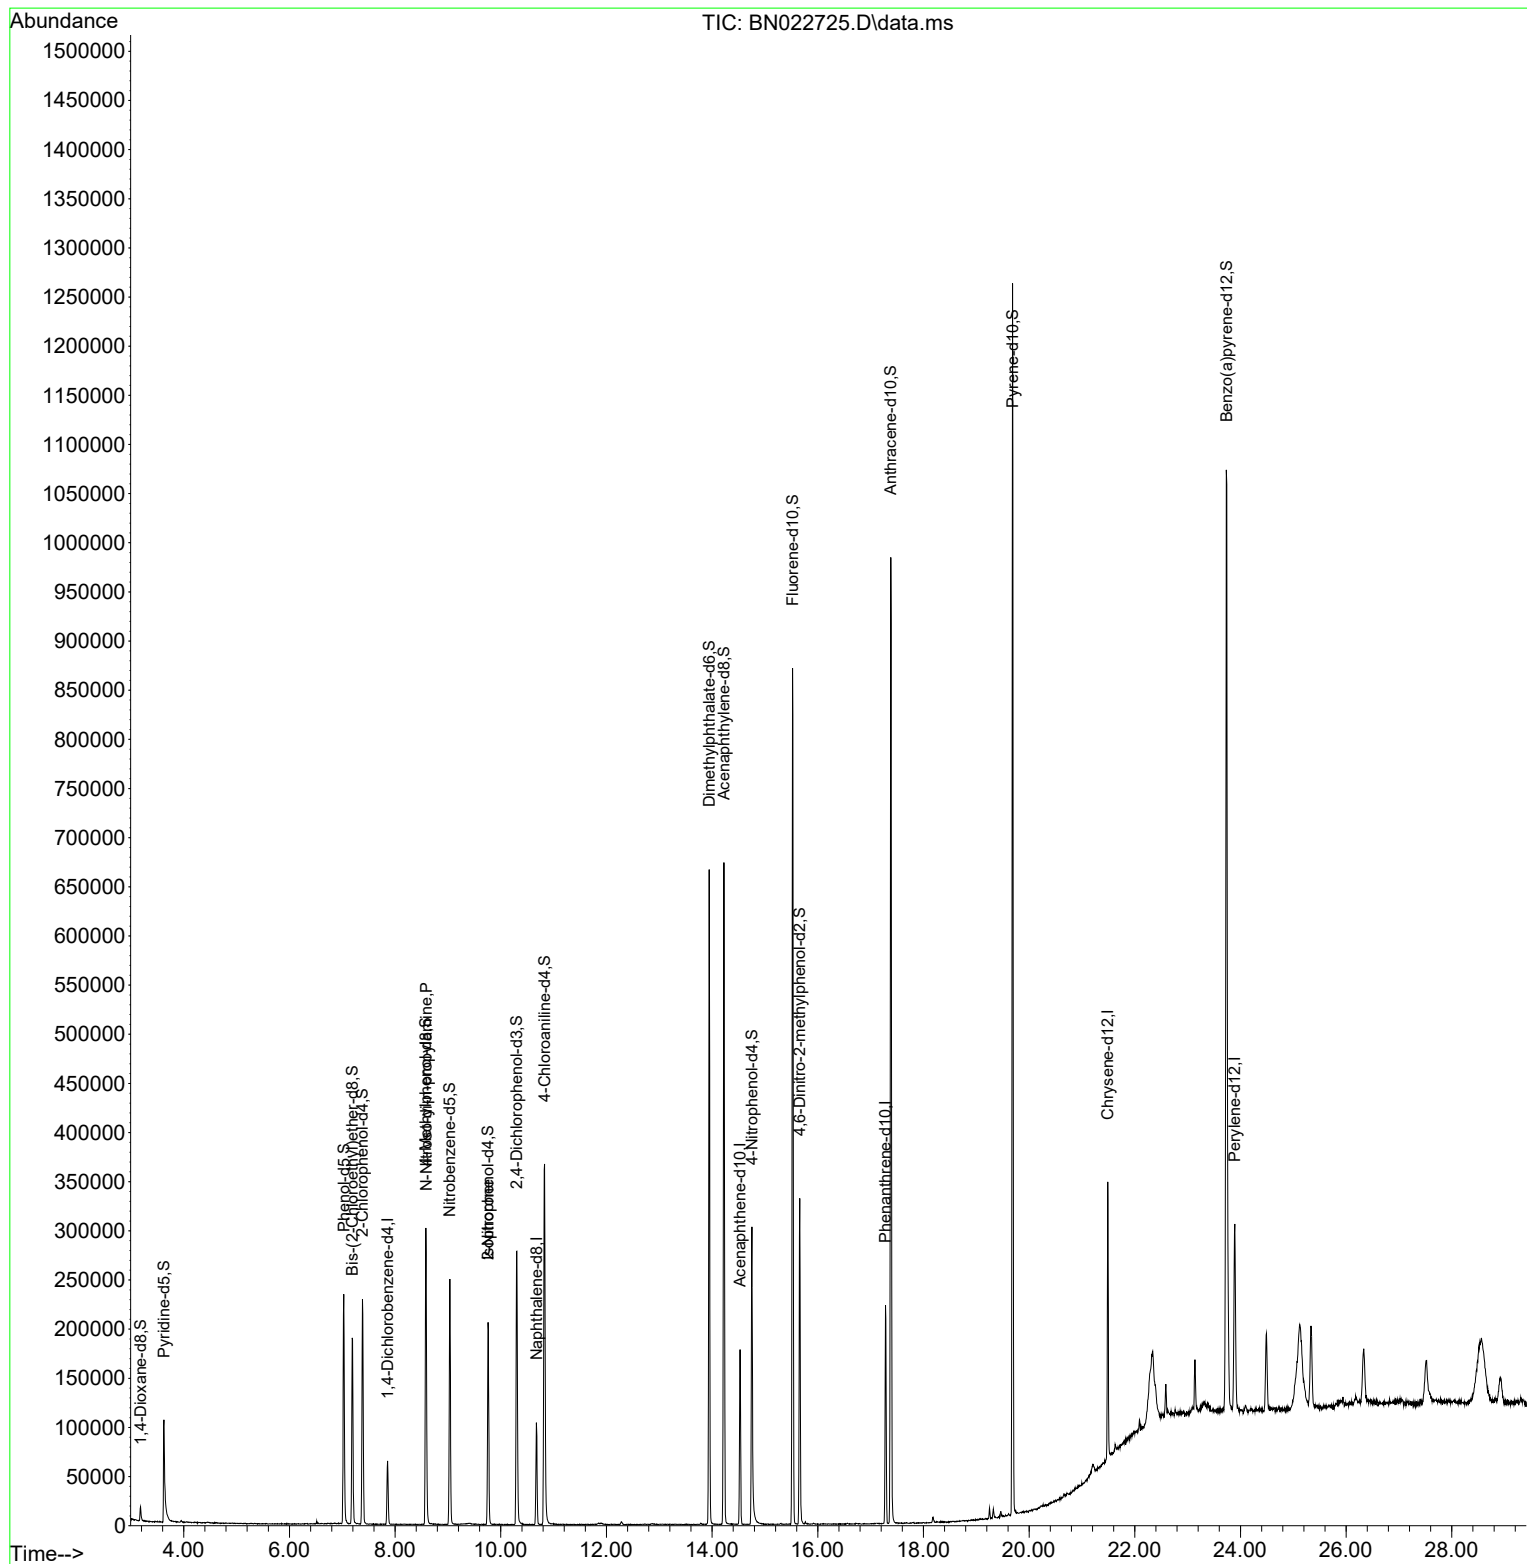


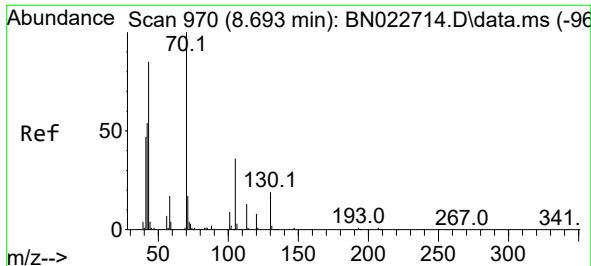

#17
N-Nitroso-di-n-propylamine
Concen: 2.917 ng/ul
RT: 8.587 min Scan# 91
Delta R.T. -0.094 min
Lab File: BN022725.D
Acq: 17 Nov 2022 18:19

Instrument :
BNA_N
ClientSampleId :
SBLK134

Tgt Ion: 70 Resp: 3018
Ion Ratio Lower Upper
70 100
42 333.5 43.4 65.2#
101 0.0 8.0 12.0#
130 0.0 16.2 24.4#

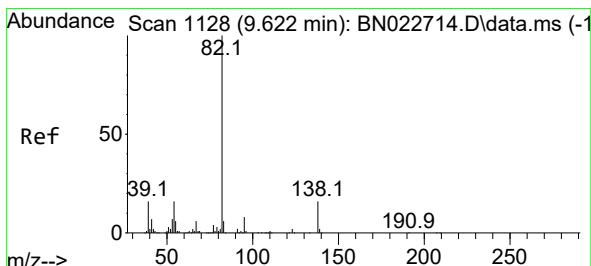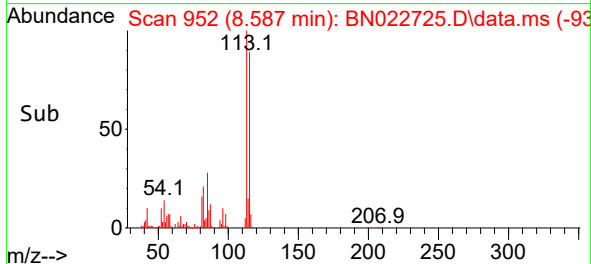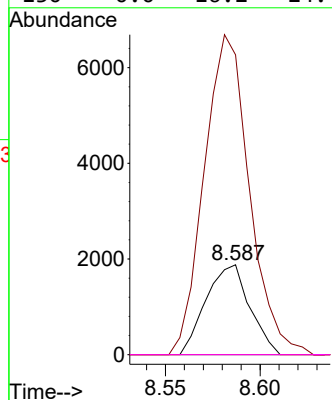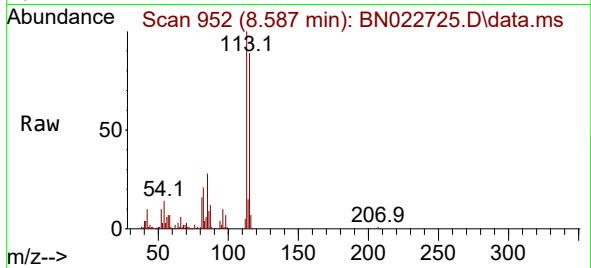

#23
Isophorone
Concen: 1.907 ng/ul
RT: 9.758 min Scan# 1151
Delta R.T. 0.153 min
Lab File: BN022725.D
Acq: 17 Nov 2022 18:19

Tgt Ion: 82 Resp: 6079
Ion Ratio Lower Upper
82 100
95 7.2 6.3 9.5
138 0.0 12.8 19.2#

