

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022746.D
 Acq On : 18 Nov 2022 08:31
 Operator : CG/JU
 Sample : PB149074BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK074

Quant Time: Nov 18 21:46:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	53018	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	258557	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	176292	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	371913	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	385072	20.000	ng/ul	0.00
88) Perylene-d12	23.886	264	394266	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	9628	6.200	ng/uL	0.00
4) Pyridine-d5	3.611	84	124877	28.435	ng/ul	0.00
7) Phenol-d5	7.016	99	153014	30.557	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	102182	34.034	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	116473	31.761	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	127753	32.316	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	62527	31.243	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	69097	30.942	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	110491	29.023	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	186612	32.181	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	440609	34.362	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	462807	32.757	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	75214	29.424	ng/ul	0.00
60) Fluorene-d10	15.522	176	363201	34.536	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	62078	26.260	ng/ul	0.00
73) Anthracene-d10	17.381	188	577251	35.446	ng/ul	0.00
81) Pyrene-d10	19.686	212	651960	32.670	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	683963	34.510	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.575	70	3484	1.036 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022746.D
Acq On : 18 Nov 2022 08:31
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK074


Quant Time: Nov 18 21:46:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

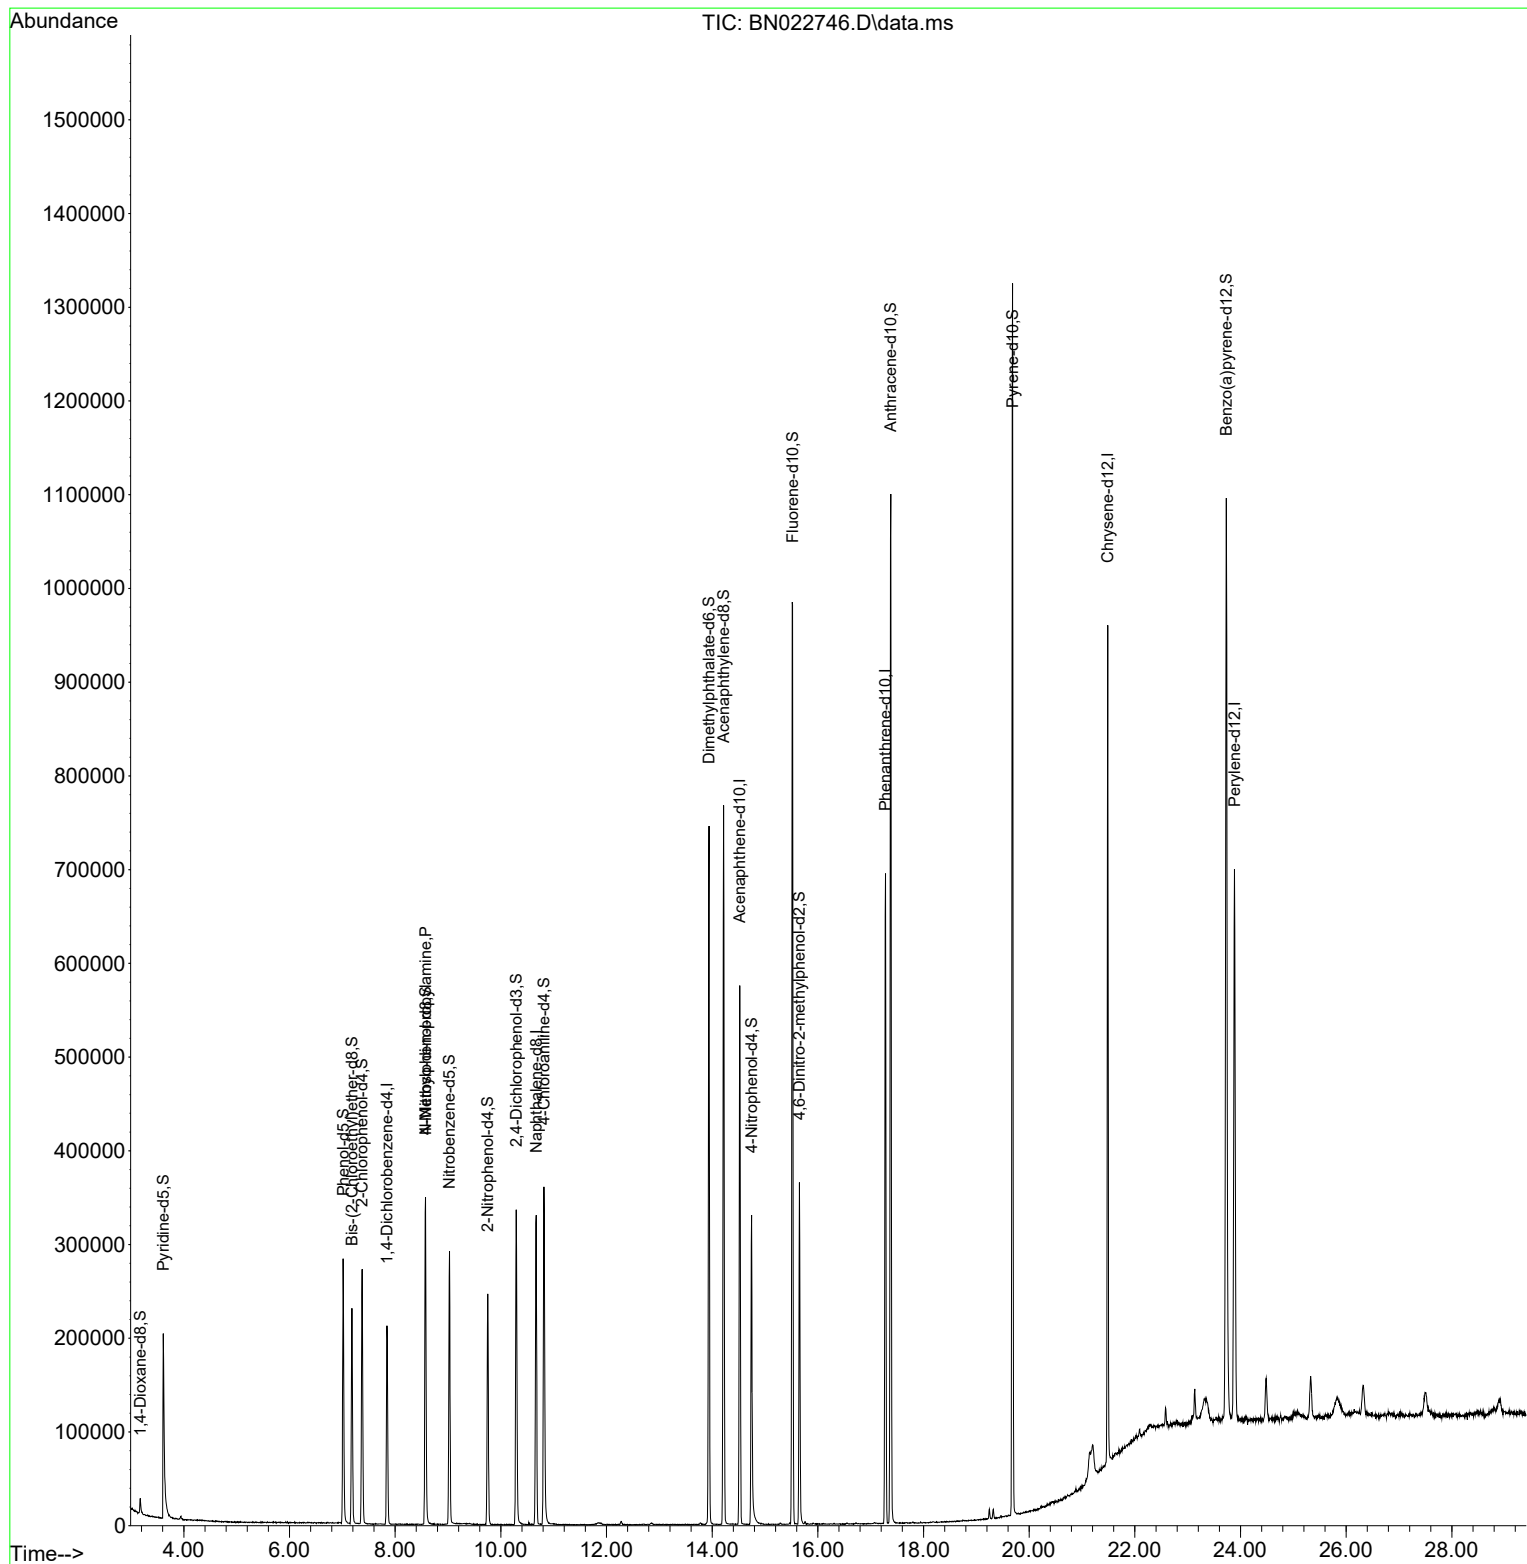

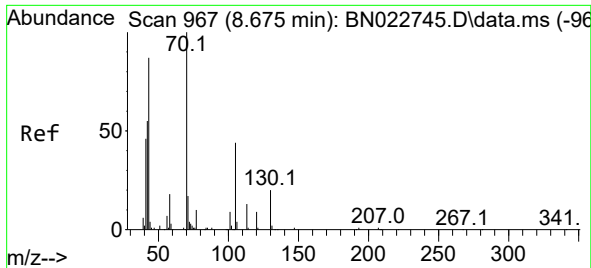

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.036 ng/ul
 RT: 8.575 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BN022746.D
 Acq: 18 Nov 2022 08:31

Instrument :
 BNA_N
 ClientSampleId :
 SBLK074

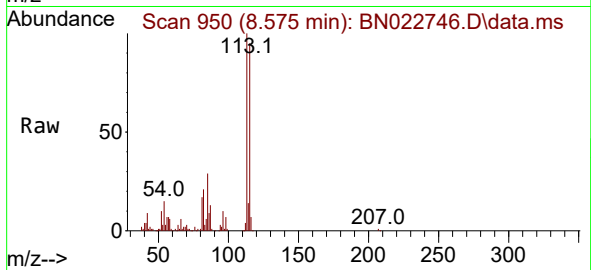

Tgt Ion: 70 Resp: 3484

Ion	Ratio	Lower	Upper
70	100		
42	347.3	43.4	65.2#
101	0.0	8.0	12.0#
130	0.0	16.2	24.4#

