




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022718.D
Acq On : 17 Nov 2022 14:00
Operator : CG/JU
Sample : N5622-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCB4

Manual IntegrationsAPPROVED

Quant Time: Nov 17 22:11:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 17 22:08:43 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/18/2022
Supervised By :mohammad ahmed 11/21/2022

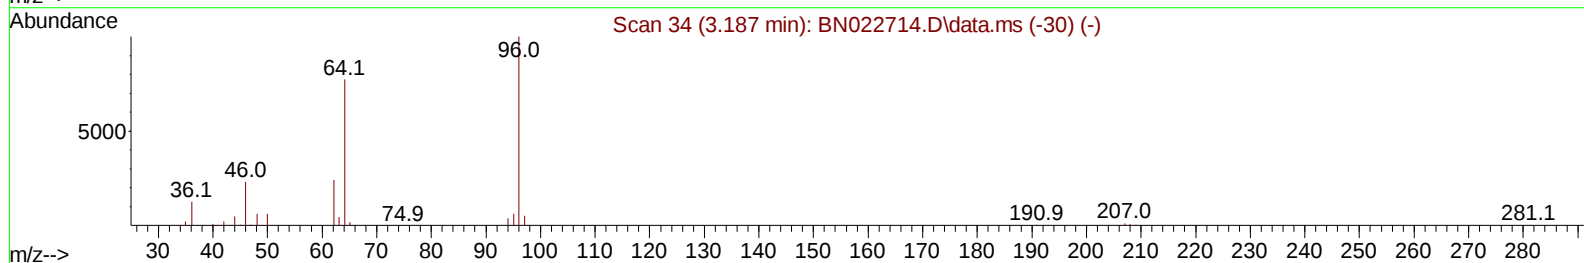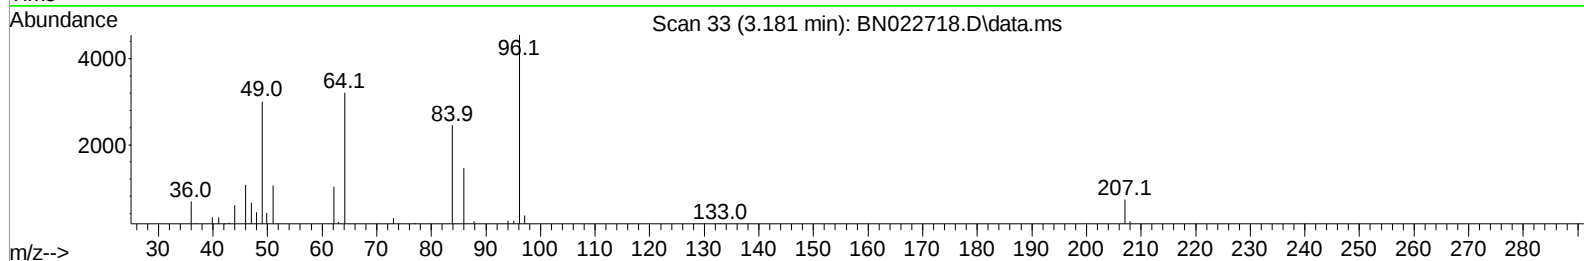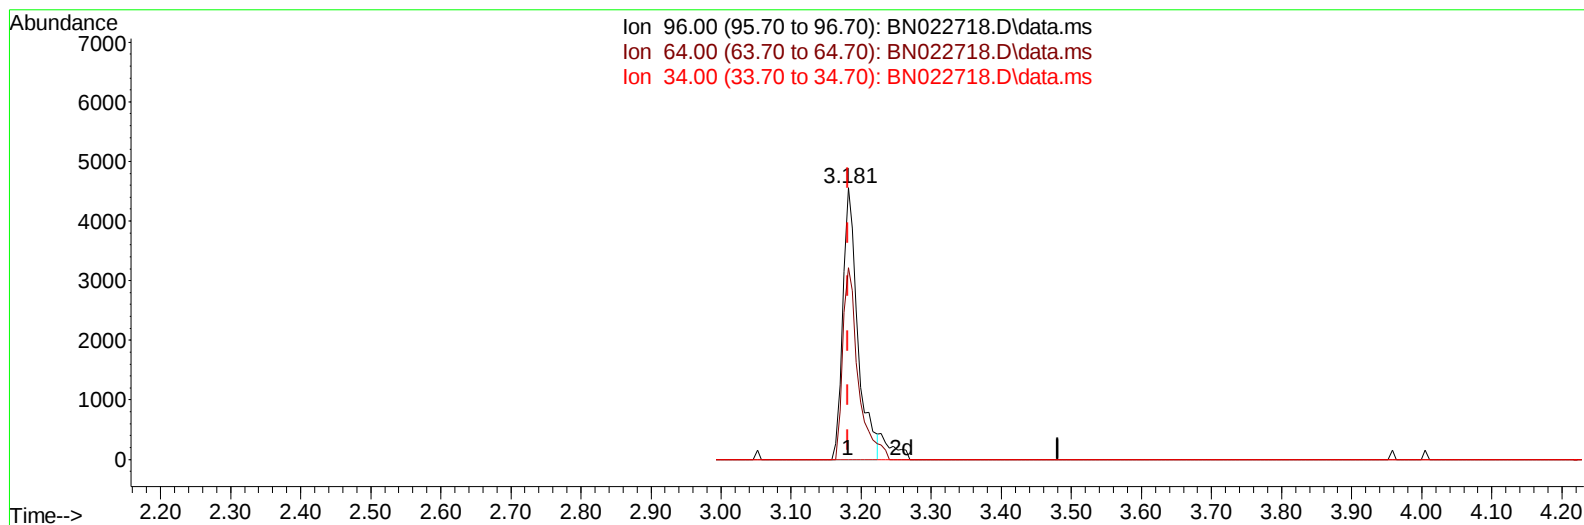

TIC: BN022718.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.000) 3.82 ng/uL

response 6803

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	70.54
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022718.D
 Acq On : 17 Nov 2022 14:00
 Operator : CG/JU
 Sample : N5622-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCB4

Manual IntegrationsAPPROVED

Quant Time: Nov 17 22:11:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/18/2022
 Supervised By :mohammad ahmed 11/21/2022

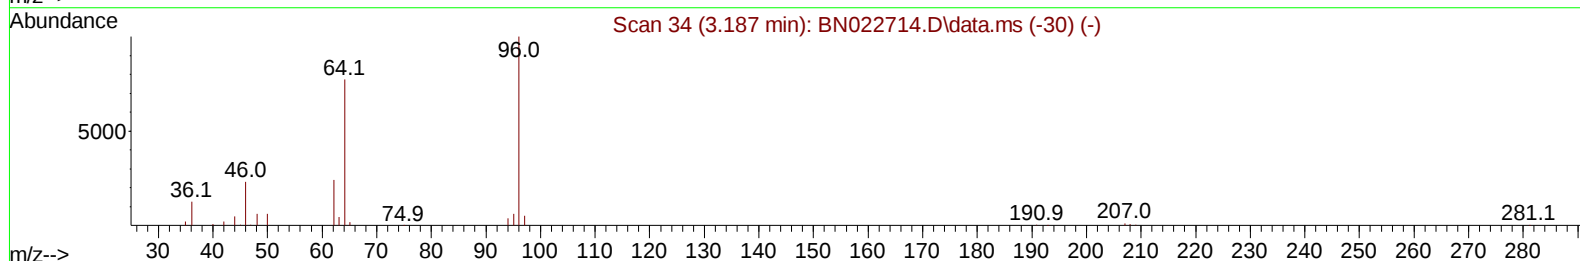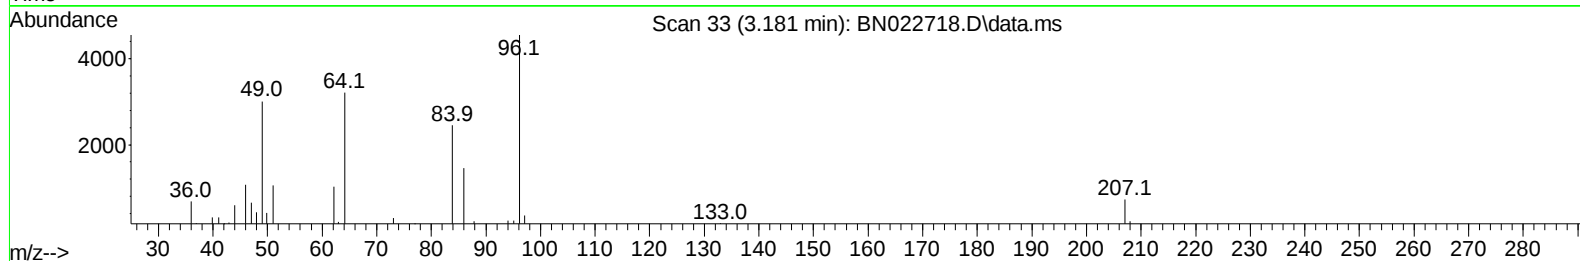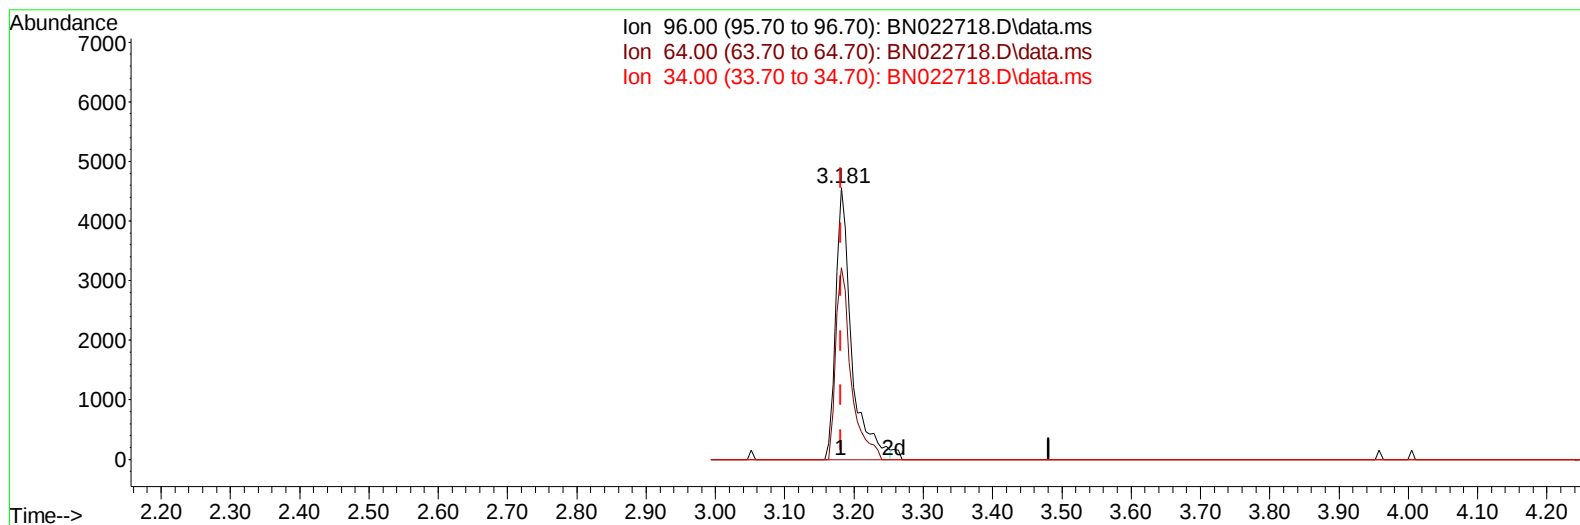

TIC: BN022718.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.000) 4.07 ng/uL m

response 7255

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	70.54
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022718.D
 Acq On : 17 Nov 2022 14:00
 Operator : CG/JU
 Sample : N5622-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCB4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/18/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 17 22:11:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	60878	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	284594	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	199147	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	419305	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	442481	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	485074	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	7255m	4.069	ng/uL	0.00
4) Pyridine-d5	3.628	84	39955	7.923	ng/ul	0.01
7) Phenol-d5	7.028	99	38607	6.715	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	114771	33.292	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	101212	24.036	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	72649	16.005	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	70303	31.914	ng/ul	0.00
24) 2-Nitrophenol-d4	9.758	143	75257	30.617	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.305	165	113810	27.160	ng/ul	0.00
31) 4-Chloroaniline-d4	10.828	131	175051	27.425	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	501618	34.630	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	526672	32.999	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	17465	6.048	ng/ul	0.00
60) Fluorene-d10	15.528	176	410248	34.532	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	77458	29.063	ng/ul	0.00
73) Anthracene-d10	17.387	188	712306	38.796	ng/ul	0.00
81) Pyrene-d10	19.692	212	814805	35.533	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	893708	36.651	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022718.D
Acq On : 17 Nov 2022 14:00
Operator : CG/JU
Sample : N5622-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGC4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/18/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 17 22:11:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 17 22:08:43 2022
Response via : Initial Calibration

