




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022726.D
 Acq On : 17 Nov 2022 18:56
 Operator : CG/JU
 Sample : N5622-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCA2

Manual IntegrationsAPPROVED

Quant Time: Nov 17 22:12:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/18/2022
 Supervised By :mohammad ahmed 11/21/2022

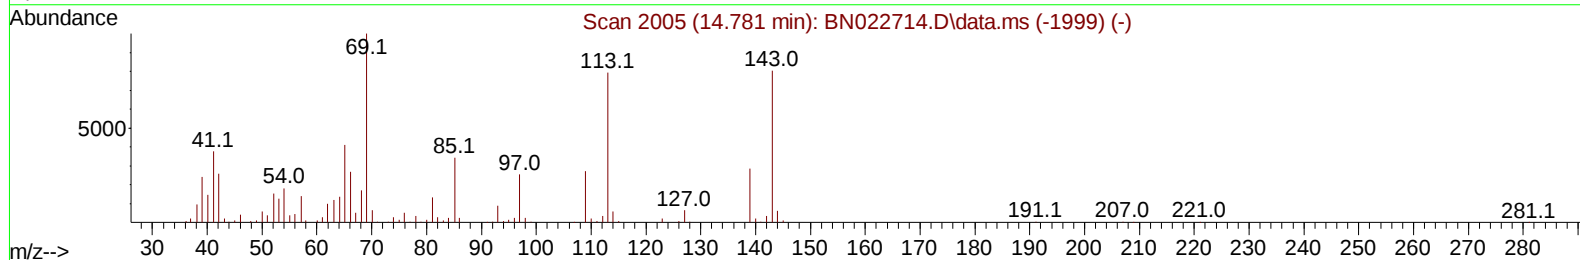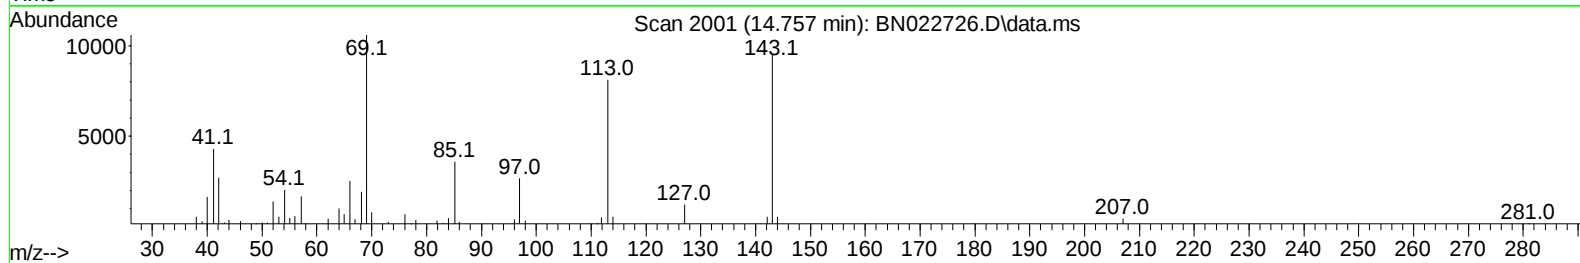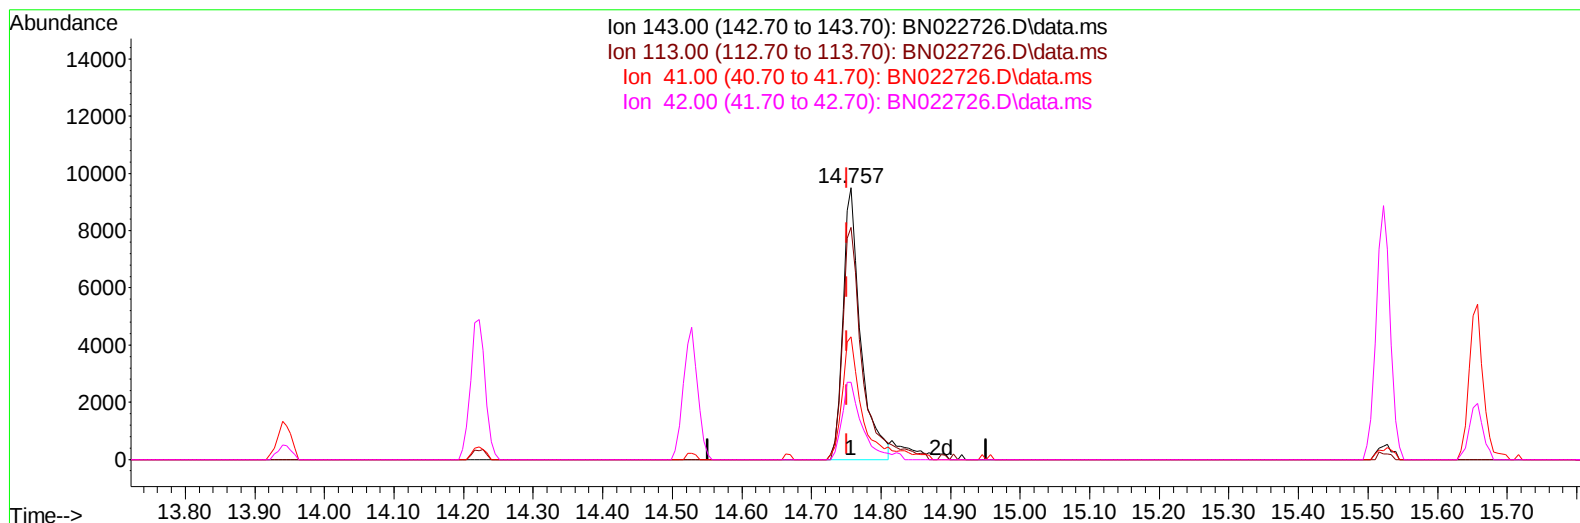

TIC: BN022726.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 6.40 ng/u1

response 16660

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	85.51
41.00	46.30	45.13
42.00	31.30	28.45




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022726.D
 Acq On : 17 Nov 2022 18:56
 Operator : CG/JU
 Sample : N5622-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCA2

Manual IntegrationsAPPROVED

Quant Time: Nov 17 22:12:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/18/2022
 Supervised By :mohammad ahmed 11/21/2022

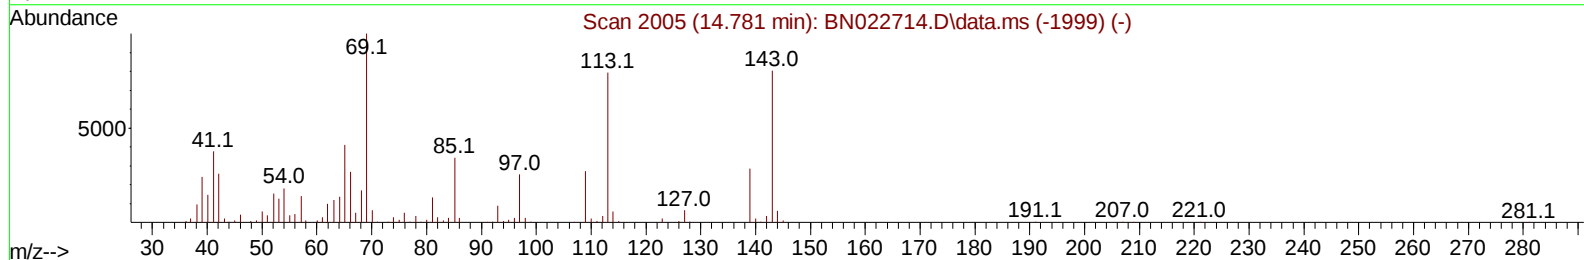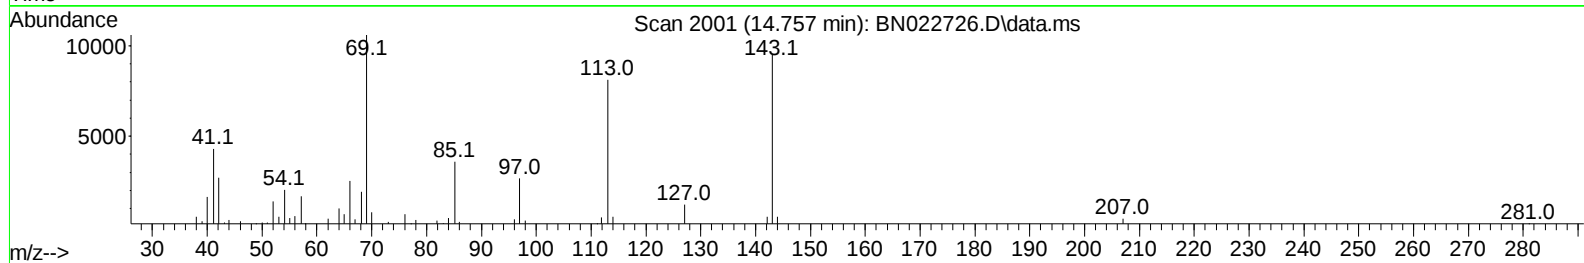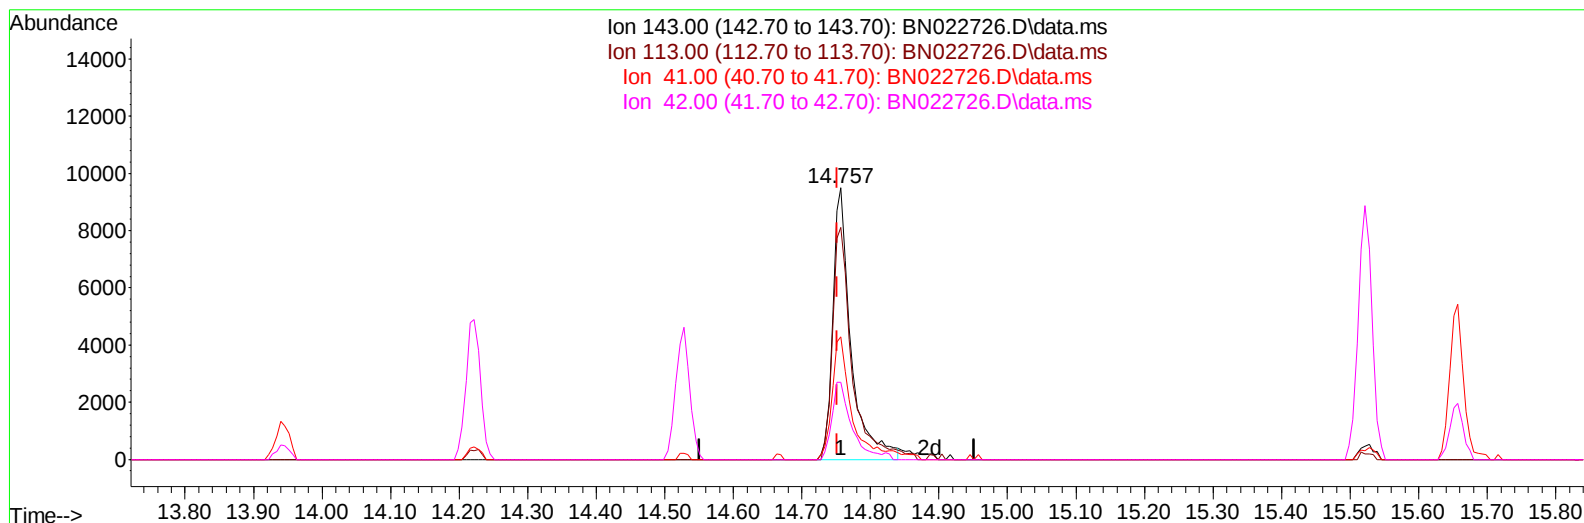

TIC: BN022726.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 6.72 ng/ul m

response 17508

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	85.51
41.00	46.30	45.13
42.00	31.30	28.45

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022726.D
 Acq On : 17 Nov 2022 18:56
 Operator : CG/JU
 Sample : N5622-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCA2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/18/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 17 22:12:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 17 22:08:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	52588	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	252030	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	179630	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	384271	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	401792	20.000	ng/ul	0.00
88) Perylene-d12	23.886	264	425421	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	6831	4.435	ng/uL	0.00
4) Pyridine-d5	3.628	84	30967	7.109	ng/ul	0.01
7) Phenol-d5	7.028	99	38467	7.745	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	109844	36.886	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	99512	27.358	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	72566	18.506	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	66640	34.160	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143	70784	32.519	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	110986	29.908	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	170155	30.103	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	474794	36.339	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	498702	34.641	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	17508m	6.722	ng/ul	0.00
60) Fluorene-d10	15.522	176	403039	37.612	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	74668	30.570	ng/ul	0.00
73) Anthracene-d10	17.381	188	665151	39.530	ng/ul	0.00
81) Pyrene-d10	19.686	212	764177	36.700	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	810757	37.912	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022726.D
Acq On : 17 Nov 2022 18:56
Operator : CG/JU
Sample : N5622-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCA2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/18/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 17 22:12:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 17 22:08:43 2022
Response via : Initial Calibration

