




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022757.D
Acq On : 18 Nov 2022 15:13
Operator : CG/JU
Sample : N5689-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:48:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

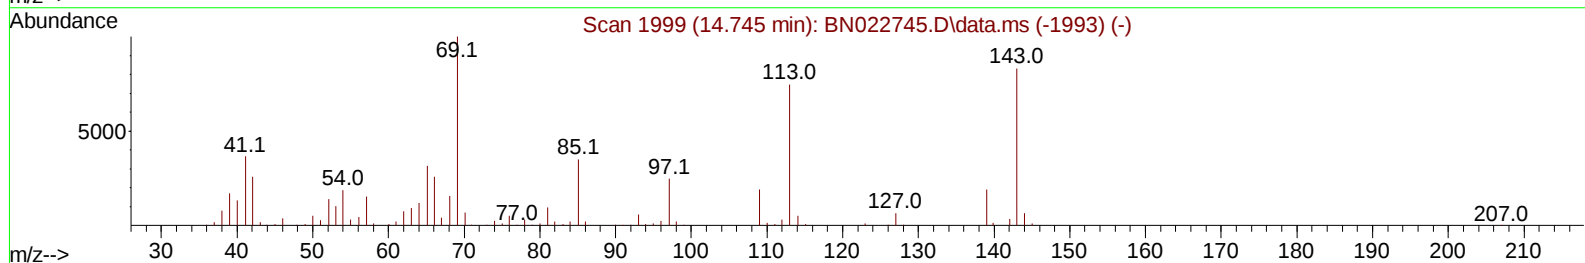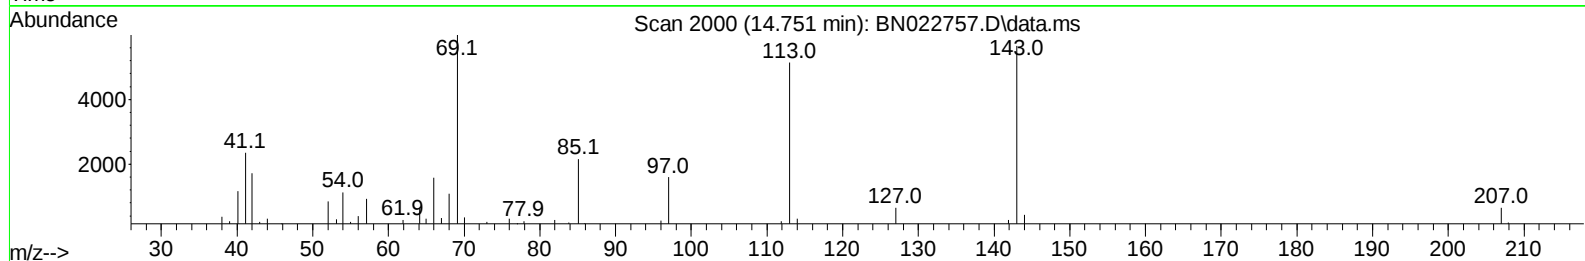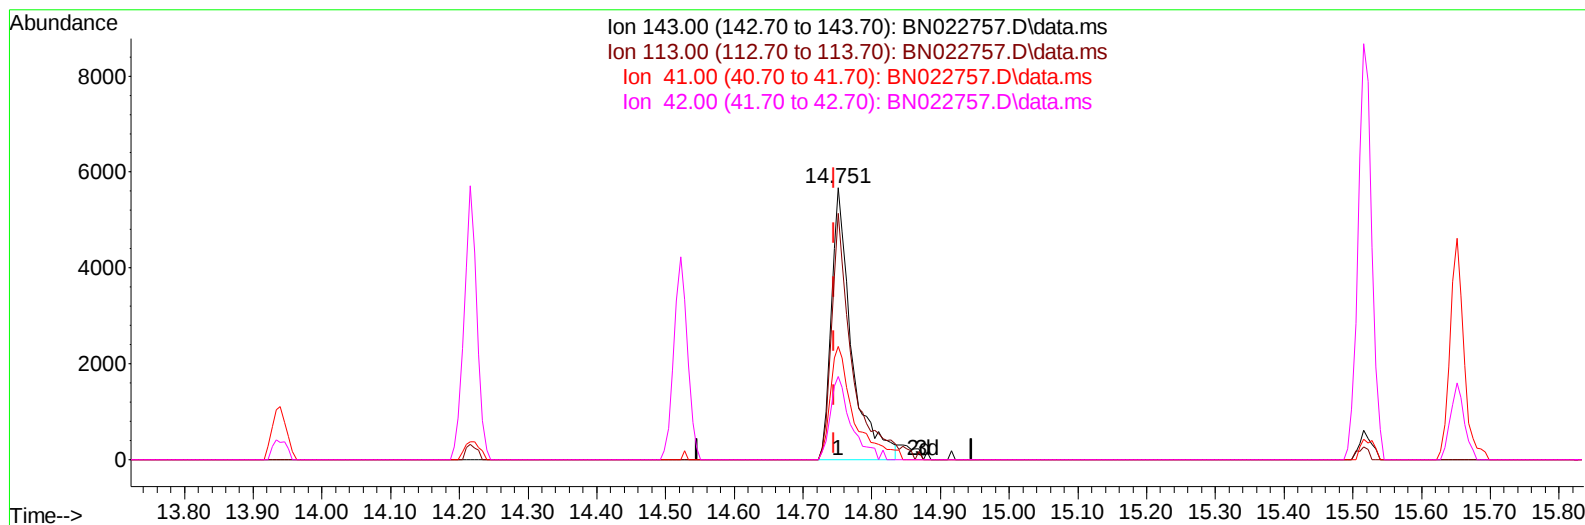

TIC: BN022757.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 5.02 ng/ul m

response 11515

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	90.68
41.00	46.30	41.52
42.00	31.30	30.49

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022757.D
 Acq On : 18 Nov 2022 15:13
 Operator : CG/JU
 Sample : N5689-09
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:48:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	46725	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	228930	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	158119	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	336303	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	349689	20.000	ng/ul	0.00
88) Perylene-d12	23.886	264	385510	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	6365	4.651	ng/uL	0.00
4) Pyridine-d5	3.628	84	28849	7.454	ng/ul	0.01
7) Phenol-d5	7.022	99	29355	6.652	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	104755	39.591	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	86939	26.900	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	61635	17.691	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	63014	35.561	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143	68200	34.493	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	103753	30.780	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	159635	31.091	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	454880	39.552	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	483478	38.153	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	11515m	5.022	ng/ul	0.00
60) Fluorene-d10	15.522	176	376448	39.909	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	60799	28.443	ng/ul	0.00
73) Anthracene-d10	17.381	188	614601	41.736	ng/ul	0.00
81) Pyrene-d10	19.686	212	679413	37.491	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	745663	38.478	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022757.D
Acq On : 18 Nov 2022 15:13
Operator : CG/JU
Sample : N5689-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:48:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

