




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111722\  
 Data File : BN022762.D  
 Acq On : 18 Nov 2022 18:18  
 Operator : CG/JU  
 Sample : PB149148BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SBLK148

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 11/21/2022  
 Supervised By : mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:49:54 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN111522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Nov 18 05:17:17 2022  
 Response via : Initial Calibration

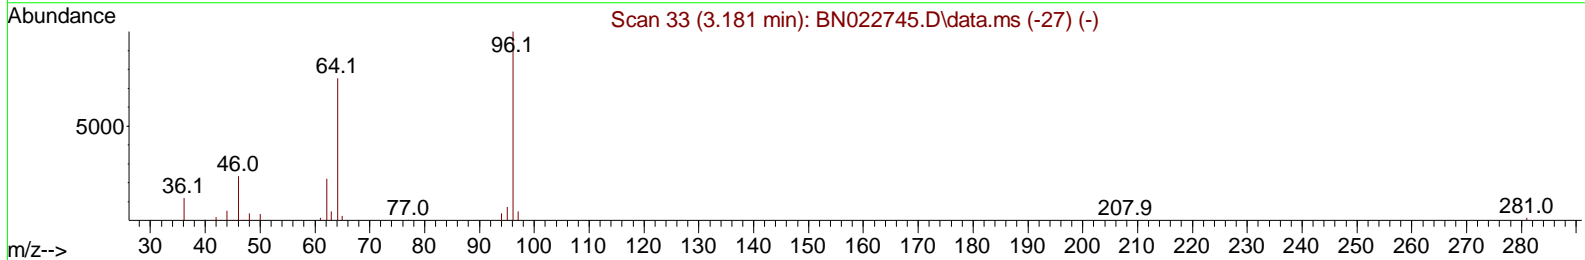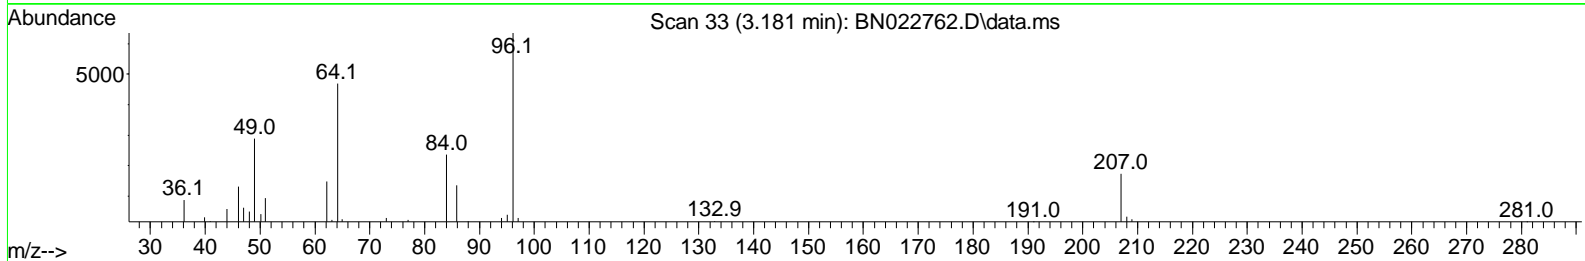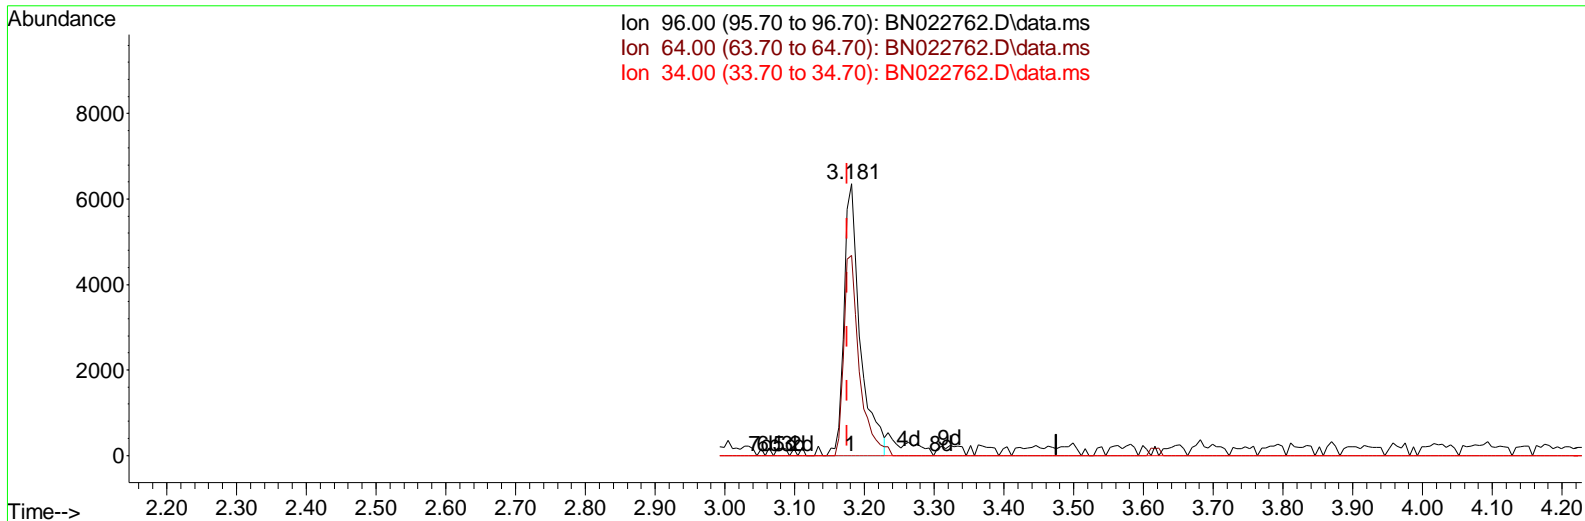

TIC: BN022762.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 6.99 ng/uL

response	10250
Ion	Exp% Act%
96.00	100.00 100.00
64.00	77.50 73.73
34.00	0.00 0.00
0.00	0.00 0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111722\  
 Data File : BN022762.D  
 Acq On : 18 Nov 2022 18:18  
 Operator : CG/JU  
 Sample : PB149148BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SBLK148

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 11/21/2022  
 Supervised By : mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:49:54 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN111522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Nov 18 05:17:17 2022  
 Response via : Initial Calibration

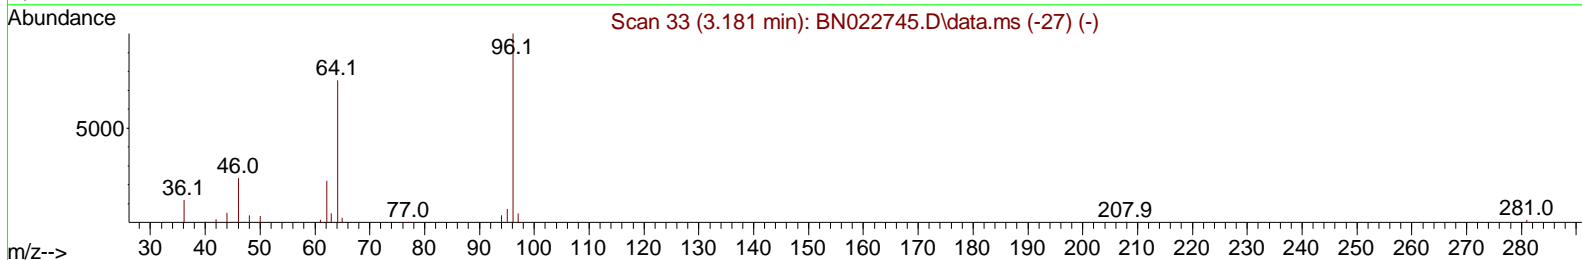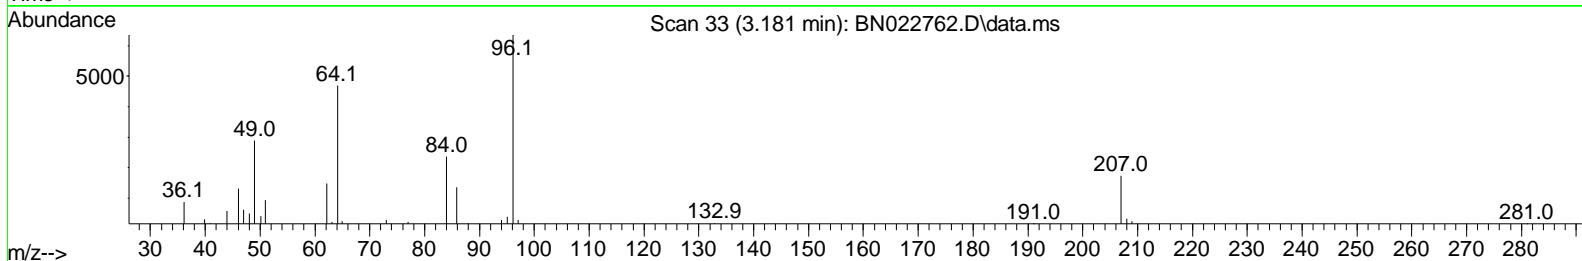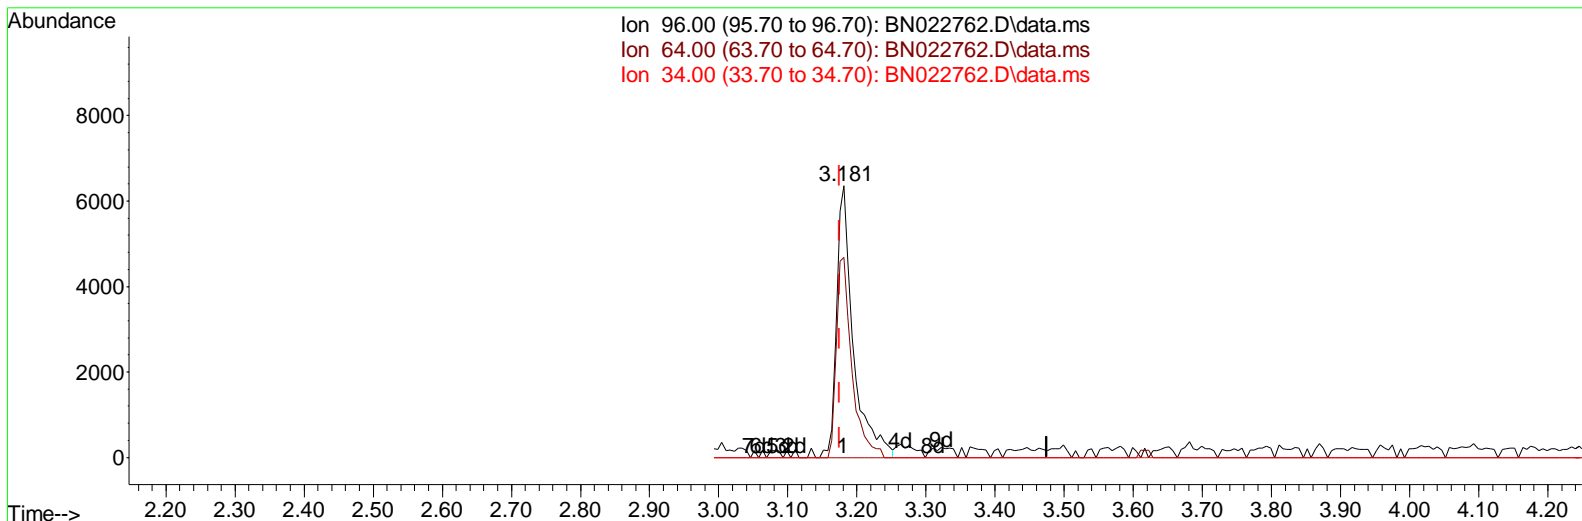

TIC: BN022762.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 7.31 ng/uL m

response	10726
Ion	Exp% Act%
96.00	100.00 100.00
64.00	77.50 73.73
34.00	0.00 0.00
0.00	0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111722\  
 Data File : BNO22762.D  
 Acq On : 18 Nov 2022 18:18  
 Operator : CG/JU  
 Sample : PB149148BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 SBLK148

**Manual Integrations APPROVED**

Reviewed By : Jagrut Upadhyay 11/21/2022  
 Supervised By : mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:49:54 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN111522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Nov 18 05:17:17 2022  
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.851	152	50074	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	242113	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	166826	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	358829	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	366564	20.000	ng/ul	0.00
88) Perylene-d12	23.886	264	374442	20.000	ng/ul	0.00
<b>System Monitoring Compounds</b>						
3) 1,4-Dioxane-d8	3.181	96	10726m	7.313	ng/uL	0.00
4) Pyridine-d5	3.616	84	138060	33.285	ng/ul	0.00
7) Phenol-d5	7.022	99	169440	35.827	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	112265	39.591	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	124678	35.998	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	138887	37.199	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	66888	35.692	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143	75148	35.937	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.298	165	123621	34.678	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	203636	37.502	ng/ul	0.00
46) Dimethylphthalate-d6	13.939	166	479434	39.511	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	504491	37.733	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	85936	35.526	ng/ul	0.00
60) Fluorene-d10	15.522	176	394674	39.658	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	68669	30.108	ng/ul	0.00
73) Anthracene-d10	17.380	188	627665	39.947	ng/ul	0.00
81) Pyrene-d10	19.686	212	712827	37.524	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	750948	39.896	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN111722\  
 Data File : BN022762.D  
 Acq On : 18 Nov 2022 18:18  
 Operator : CG/JU  
 Sample : PB149148BL  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 SBLK148

**Manual IntegrationsAPPROVED**

Reviewed By :Jagrut Upadhyay 11/21/2022  
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 21:49:54 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN111522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Nov 18 05:17:17 2022  
 Response via : Initial Calibration

