




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 22:53:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

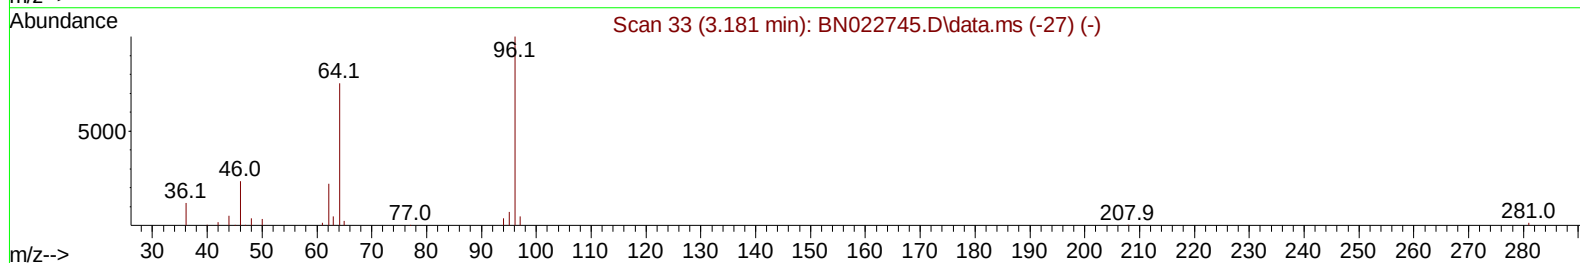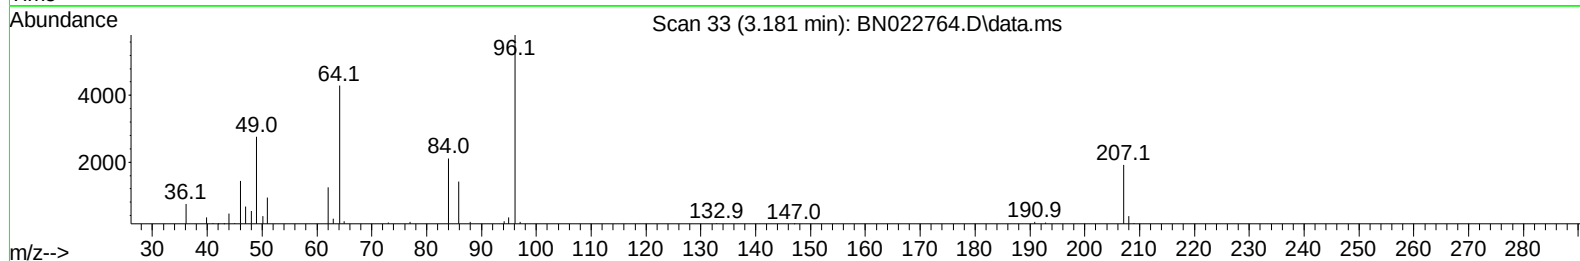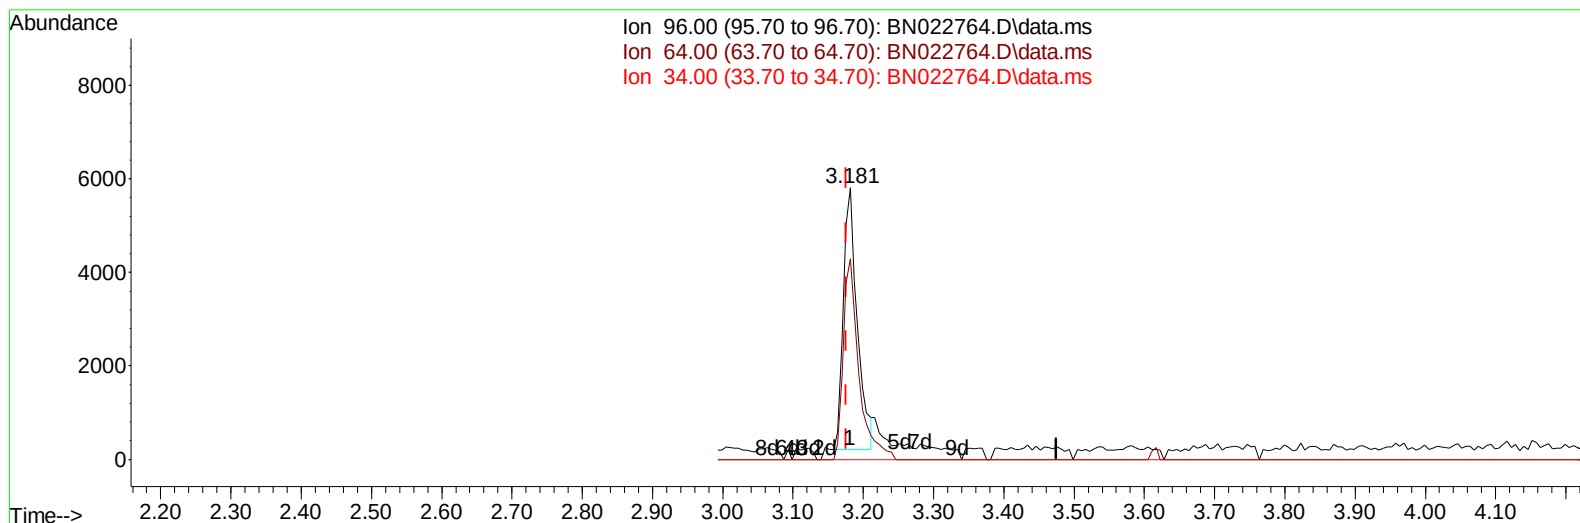

TIC: BN022764.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.181min (+ 0.006) 4.46 ng/uL****response 7694**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	73.91
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022764.D
 Acq On : 18 Nov 2022 20:10
 Operator : CG/JU
 Sample : PB149167BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK167

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:53:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

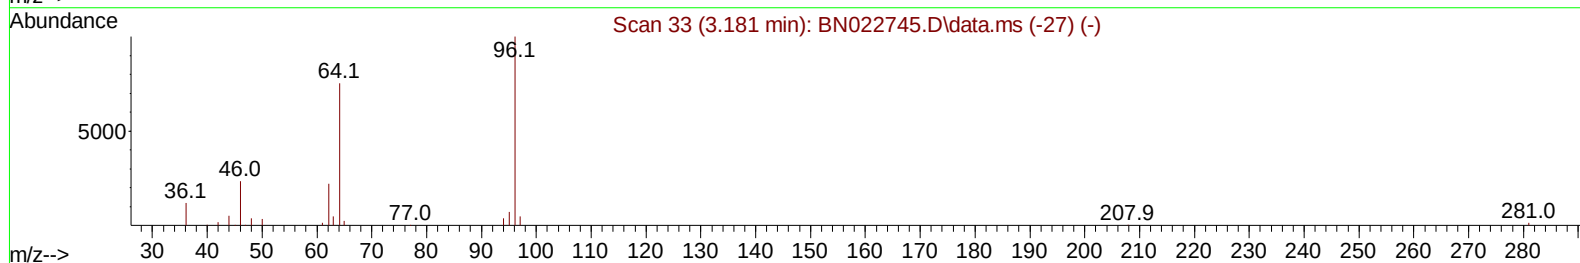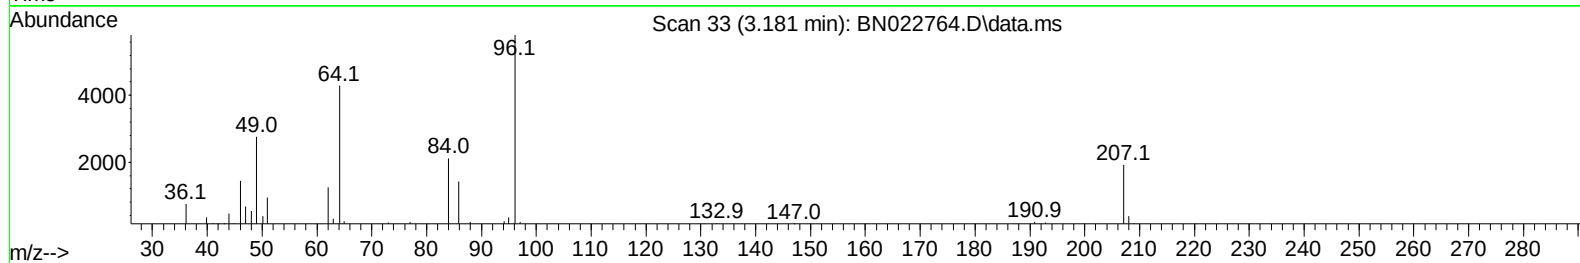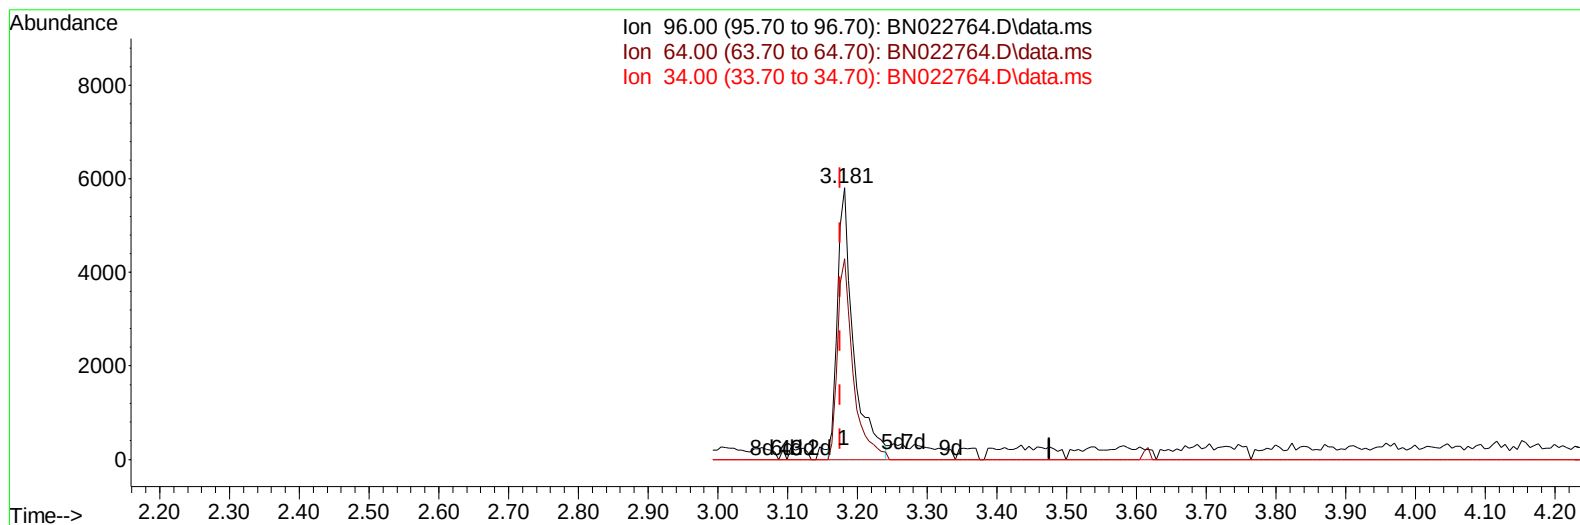

TIC: BN022764.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 5.39 ng/uL m

response 9298

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	73.91
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022764.D
 Acq On : 18 Nov 2022 20:10
 Operator : CG/JU
 Sample : PB149167BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK167

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 22:53:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	58876	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	284156	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	193566	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	421828	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	443268	20.000	ng/ul	0.00
88) Perylene-d12	23.880	264	474112	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	9298m	5.392	ng/uL	0.00
4) Pyridine-d5	3.617	84	120232	24.654	ng/ul	0.00
7) Phenol-d5	7.022	99	151360	27.220	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	100489	30.140	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	112626	27.656	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	124127	28.275	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	60552	27.530	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143	66186	26.969	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	110017	26.295	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	178566	28.019	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	430528	30.579	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	451141	29.082	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	76722	27.335	ng/ul	0.00
60) Fluorene-d10	15.522	176	349895	30.301	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	61648	22.992	ng/ul	0.00
73) Anthracene-d10	17.375	188	580280	31.416	ng/ul	0.00
81) Pyrene-d10	19.680	212	656751	28.590	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	714000	29.958	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 22:53:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

