




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022771.D
 Acq On : 19 Nov 2022 00:27
 Operator : CG/JU
 Sample : N5689-16
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 01:19:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

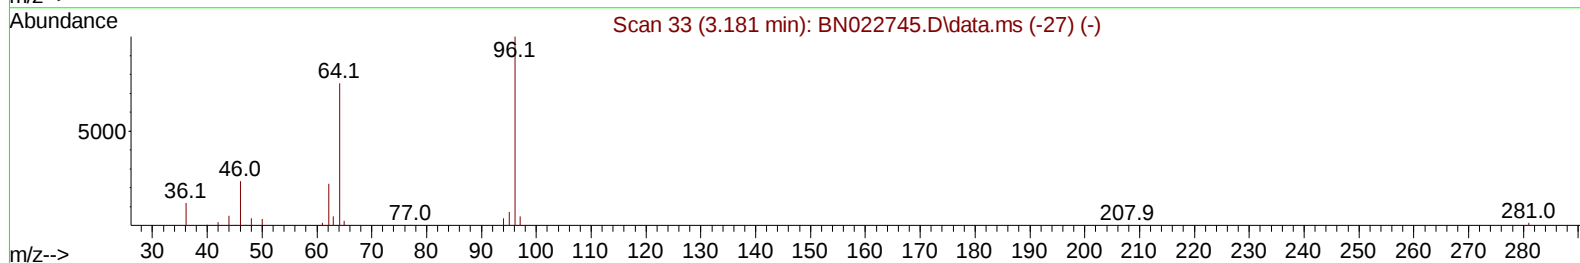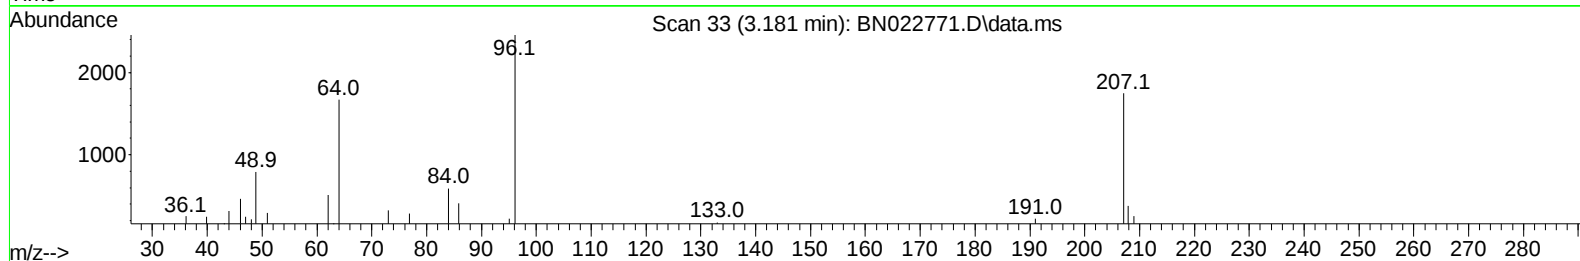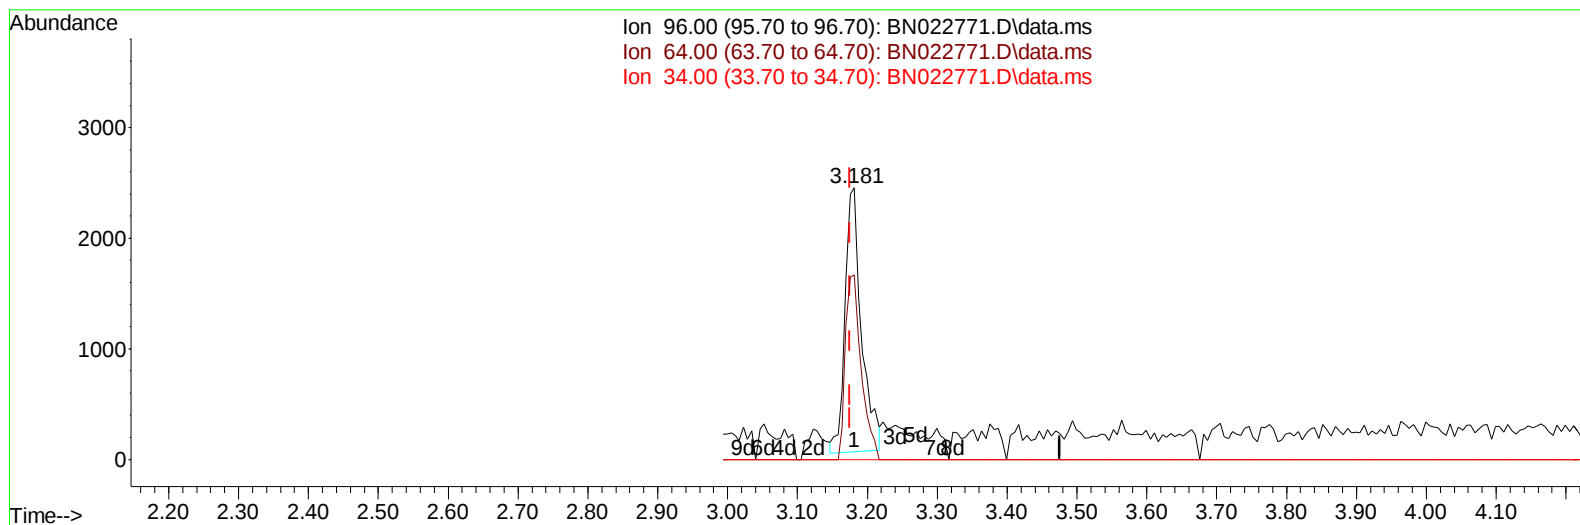

TIC: BN022771.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 2.38 ng/uL

response 3884

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	67.94
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022771.D
 Acq On : 19 Nov 2022 00:27
 Operator : CG/JU
 Sample : N5689-16
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 01:19:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

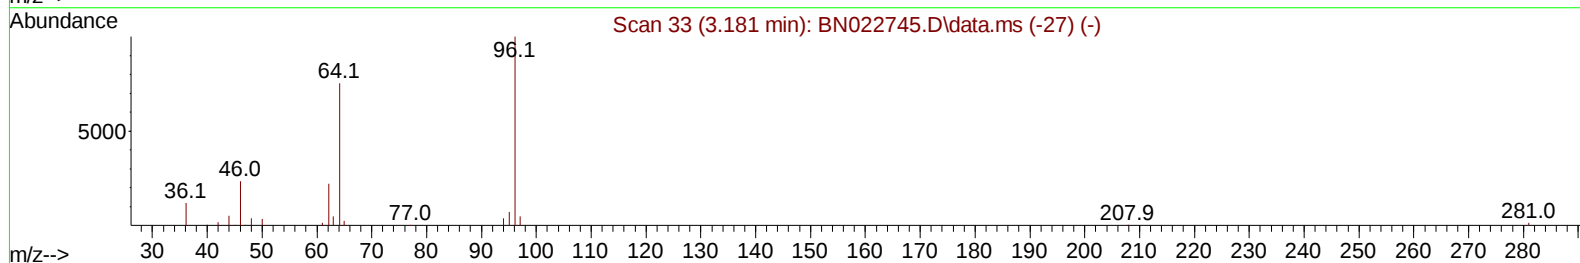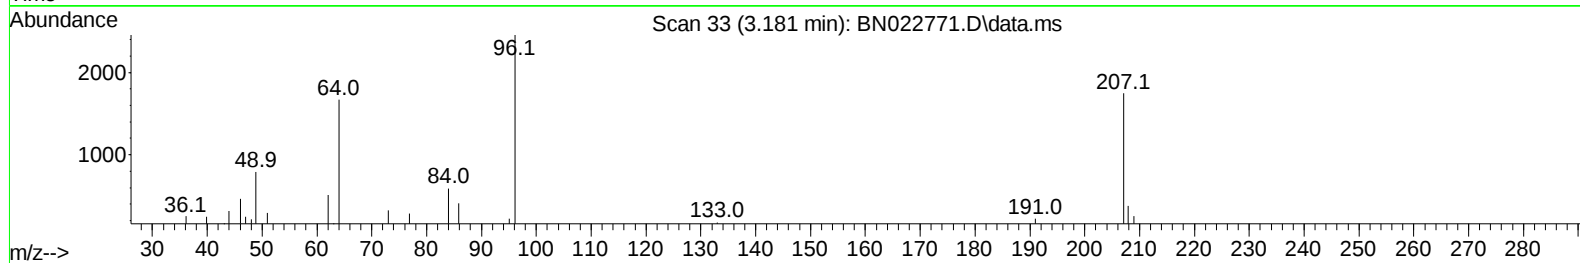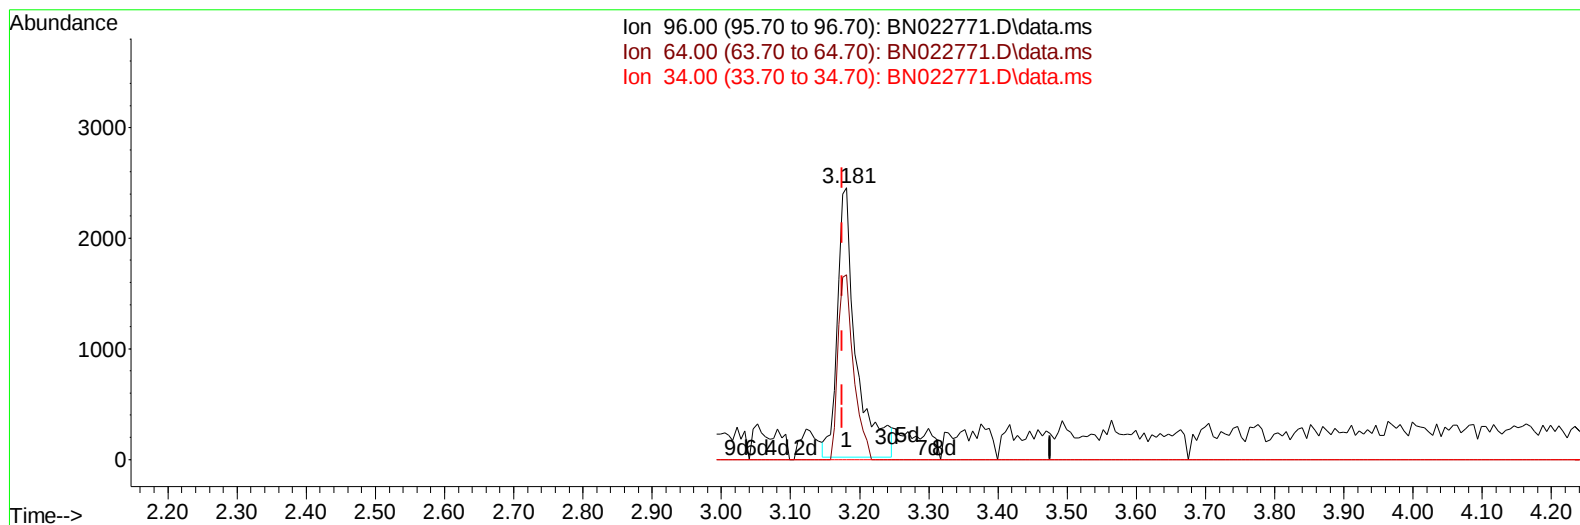

TIC: BN022771.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 2.82 ng/uL m

response 4601

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	67.94
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022771.D
 Acq On : 19 Nov 2022 00:27
 Operator : CG/JU
 Sample : N5689-16
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 01:19:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	55777	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	273963	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	188457	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	407042	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	404141	20.000	ng/ul	0.00
88) Perylene-d12	23.874	264	425117	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	4601m	2.816	ng/uL	0.00
4) Pyridine-d5	3.623	84	36891	7.985	ng/ul	0.00
7) Phenol-d5	7.022	99	35753	6.787	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	109094	34.539	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	92354	23.938	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	68823	16.548	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	66245	31.239	ng/ul	0.00
24) 2-Nitrophenol-d4	9.758	143	68578	28.983	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	110303	27.345	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	176478	28.722	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	508820	37.120	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	534451	35.386	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	21198	7.757	ng/ul	0.00
60) Fluorene-d10	15.516	176	444773	39.562	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	77678	30.023	ng/ul	0.00
73) Anthracene-d10	17.375	188	736934	41.346	ng/ul	0.00
81) Pyrene-d10	19.681	212	846076	40.397	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	886375	41.477	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022771.D
Acq On : 19 Nov 2022 00:27
Operator : CG/JU
Sample : N5689-16
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 01:19:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

