




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022774.D
Acq On : 19 Nov 2022 02:17
Operator : CG/JU
Sample : N5689-19
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 02:56:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

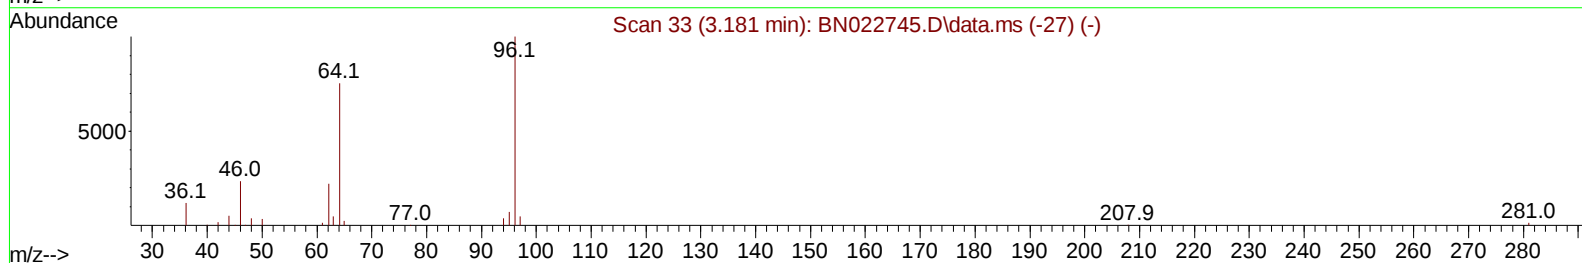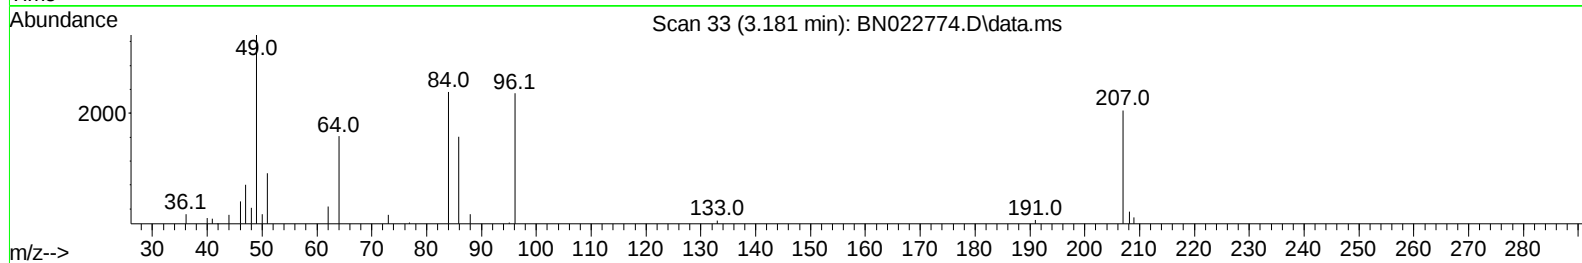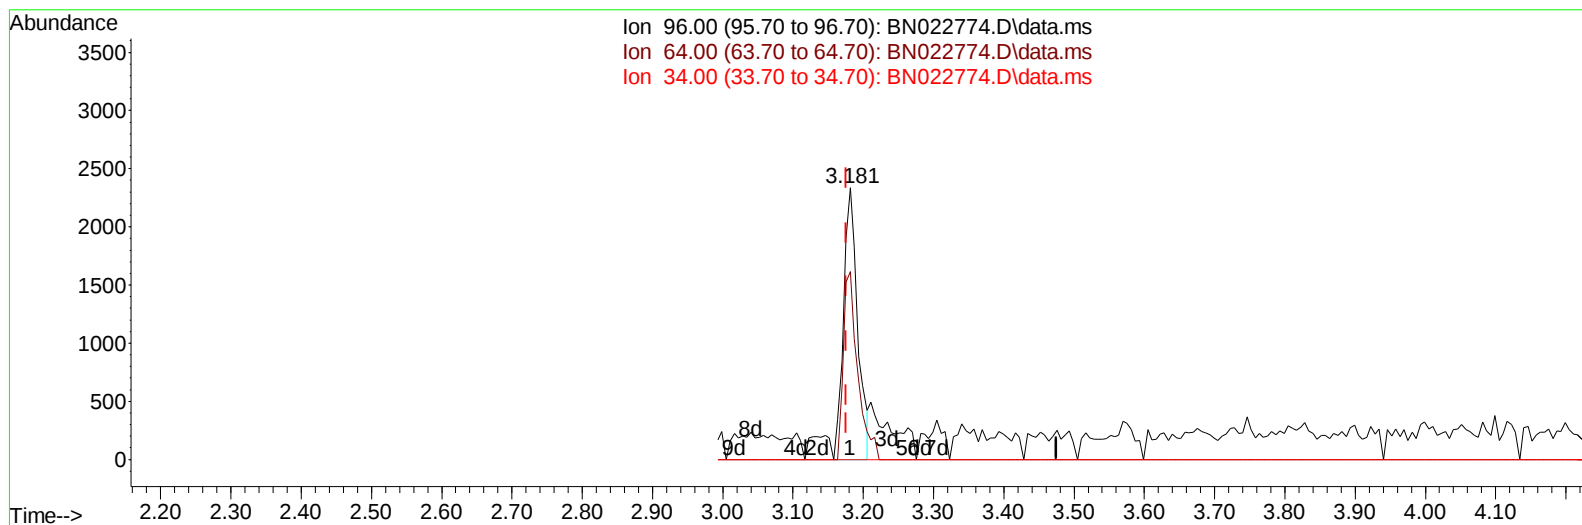

TIC: BN022774.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.181min (+ 0.006) 1.73 ng/uL****response 3241**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	69.12
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022774.D
 Acq On : 19 Nov 2022 02:17
 Operator : CG/JU
 Sample : N5689-19
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 02:56:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

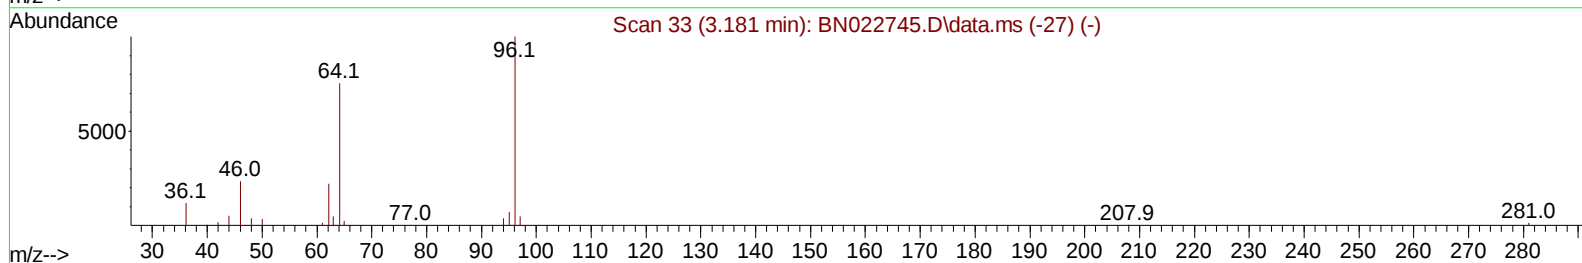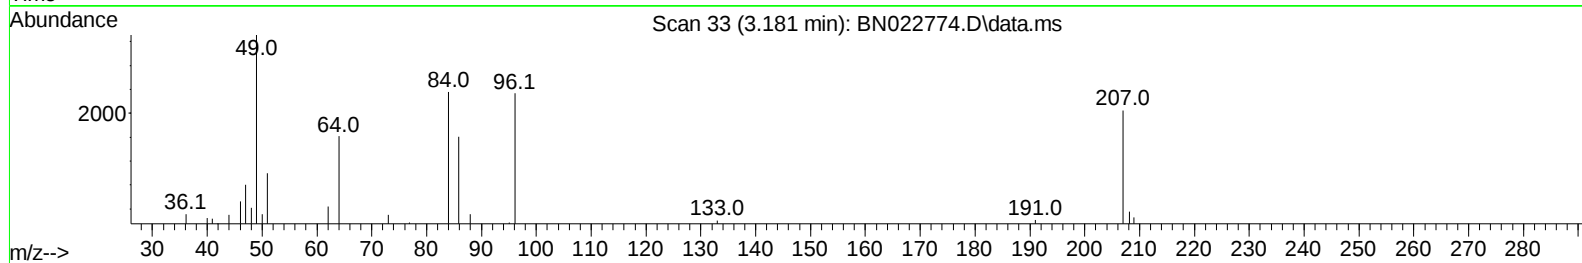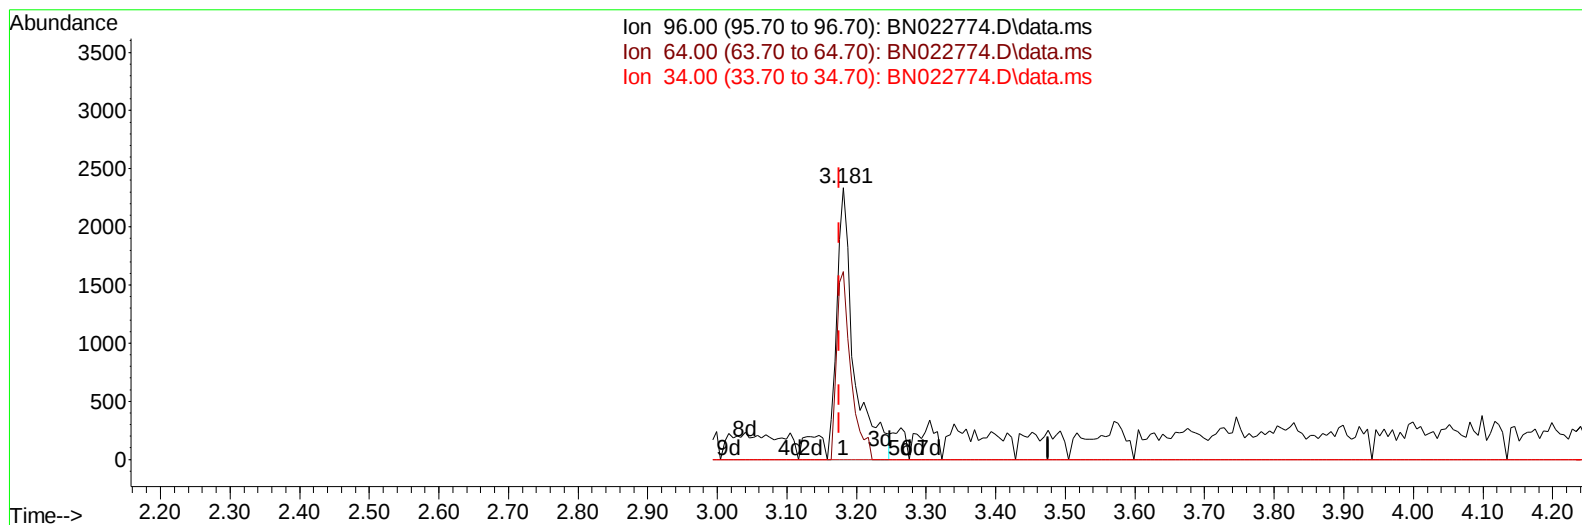

TIC: BN022774.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (+ 0.006) 2.15 ng/uL m

response 4016

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	69.12
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022774.D
 Acq On : 19 Nov 2022 02:17
 Operator : CG/JU
 Sample : N5689-19
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 02:56:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	63907	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	306322	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	207318	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	436782	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	440222	20.000	ng/ul	0.00
88) Perylene-d12	23.874	264	434900	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	4016m	2.145	ng/uL	0.00
4) Pyridine-d5	3.622	84	38730	7.316	ng/ul	0.00
7) Phenol-d5	7.022	99	33151	5.492	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	109728	30.320	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	93268	21.100	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	67123	14.086	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	67272	28.372	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	68634	25.942	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	110868	24.581	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	155751	22.671	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	500144	33.167	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	515350	31.017	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	14779	4.916	ng/ul	0.00
60) Fluorene-d10	15.516	176	414935	33.550	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	68376	24.629	ng/ul	0.00
73) Anthracene-d10	17.375	188	690439	36.100	ng/ul	0.00
81) Pyrene-d10	19.680	212	786252	34.464	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.721	264	793080	36.277	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022774.D
Acq On : 19 Nov 2022 02:17
Operator : CG/JU
Sample : N5689-19
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 02:56:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

