




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 03:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

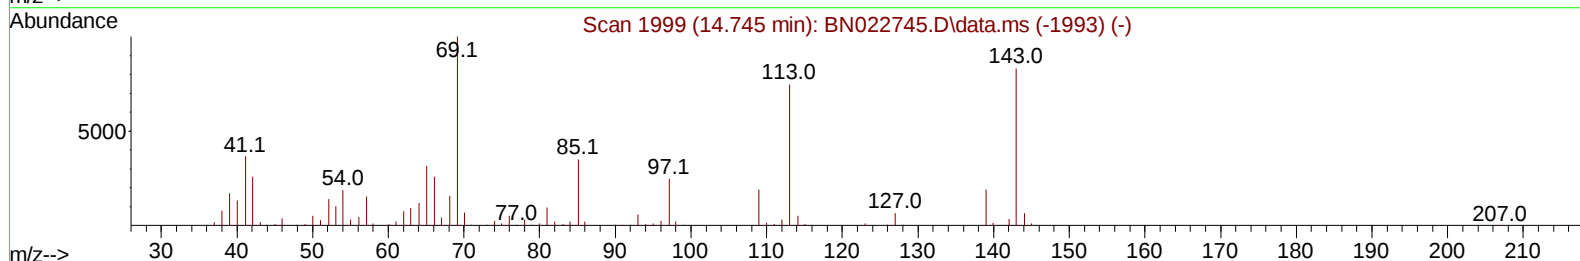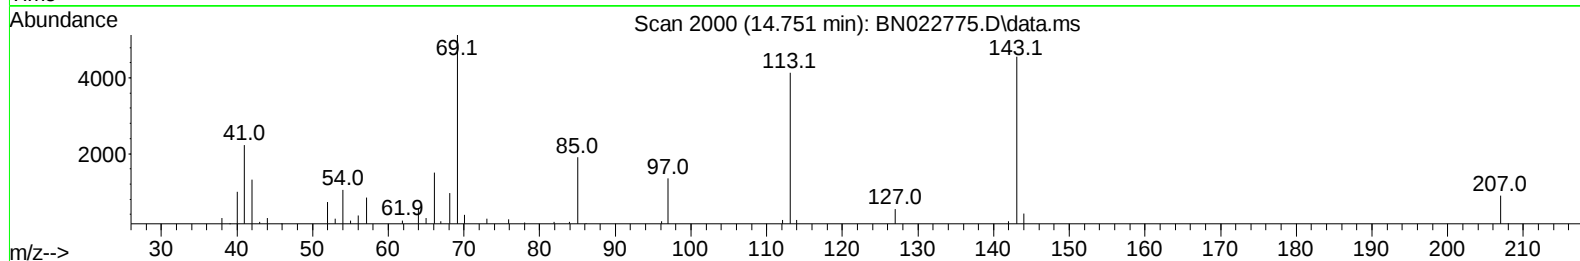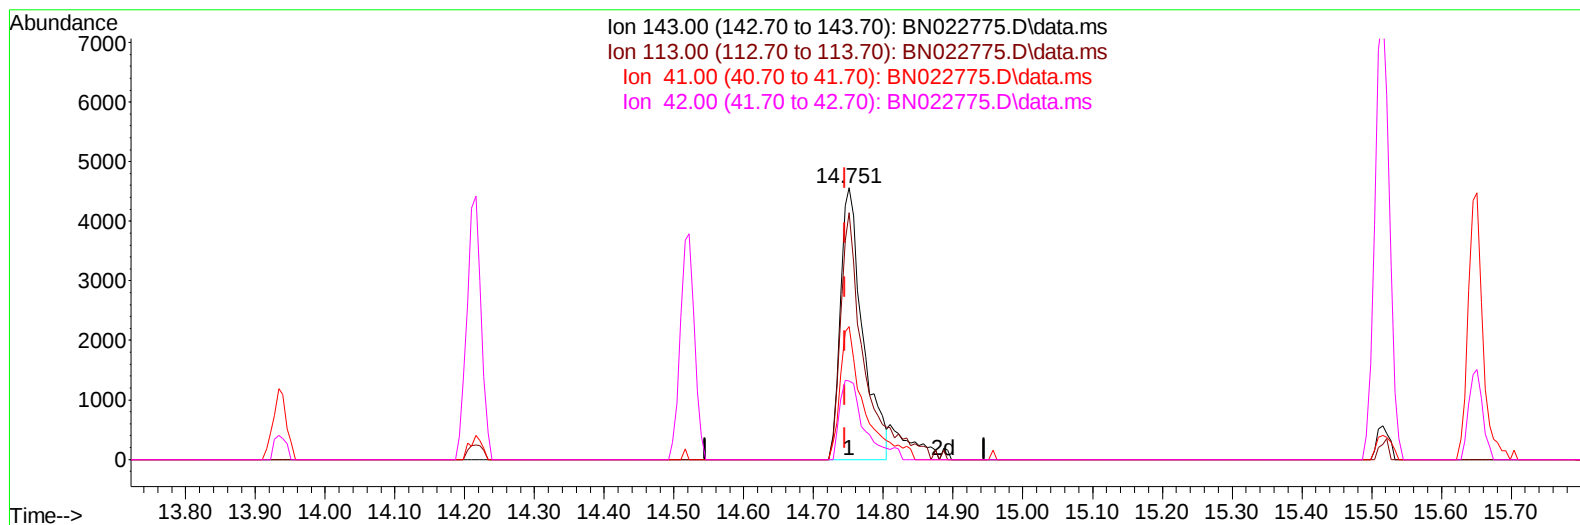

TIC: BN022775.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 4.69 ng/u1

response 10071

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	95.00	90.92
41.00	46.30	48.95
42.00	31.30	28.96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022775.D
 Acq On : 19 Nov 2022 02:53
 Operator : CG/JU
 Sample : N5689-20
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 03:34:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 18 05:17:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	44793	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	217402	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	148071	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.275	188	317402	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	316907	20.000	ng/ul	-0.01
88) Perylene-d12	23.874	264	324127	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	3675	2.801	ng/uL	0.00
4) Pyridine-d5	3.622	84	32977	8.888	ng/ul	0.00
7) Phenol-d5	7.022	99	26725	6.317	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	93356	36.804	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	77730	25.088	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	53404	15.990	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	56572	33.618	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143	57310	30.522	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	90367	28.231	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	143803	29.493	ng/ul	0.00
46) Dimethylphthalate-d6	13.939	166	412751	38.324	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	433000	36.488	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	10921m	5.087	ng/ul	0.00
60) Fluorene-d10	15.516	176	352624	39.920	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	59398	29.442	ng/ul	0.00
73) Anthracene-d10	17.375	188	611212	43.977	ng/ul	0.00
81) Pyrene-d10	19.680	212	693083	42.202	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.715	264	736440	45.198	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 03:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 18 05:17:17 2022
Response via : Initial Calibration

