

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022724.D
 Acq On : 17 Nov 2022 17:41
 Operator : CG/JU
 Sample : PB149132BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	42	rVB	13721	19409	1.04%	0.118%
2	3.622	106	108	130	rBV	90652	170651	9.14%	1.036%
3	3.952	160	164	169	rVB2	3325	4618	0.25%	0.028%
4	7.028	681	687	698	rVV	223117	356601	19.10%	2.166%
5	7.193	709	715	726	rBV	187985	297736	15.95%	1.808%
6	7.387	741	748	757	rBV	217596	356722	19.10%	2.167%
7	7.858	821	828	839	rVB	185206	293022	15.69%	1.780%
8	8.581	945	951	964	rBV	280428	470755	25.21%	2.859%
9	9.040	1021	1029	1042	rBV	226848	387661	20.76%	2.354%
10	9.763	1145	1152	1165	rVB	201457	330495	17.70%	2.007%
11	10.304	1237	1244	1259	rBV	273692	466667	24.99%	2.834%
12	10.675	1300	1307	1315	rBV	290318	475510	25.47%	2.888%
13	10.828	1326	1333	1352	rBV	218207	395260	21.17%	2.401%
14	12.287	1577	1581	1588	rVB2	3131	5356	0.29%	0.033%
15	13.787	1832	1836	1844	rVB2	1797	2995	0.16%	0.018%
16	13.945	1852	1863	1875	rBV	621631	864946	46.32%	5.253%
17	14.222	1904	1910	1924	rBV	630083	919058	49.22%	5.582%
18	14.528	1956	1962	1972	rVB	498907	706452	37.84%	4.291%
19	14.751	1994	2000	2020	rBV	281780	456755	24.46%	2.774%
20	14.875	2020	2021	2028	rVB5	1208	2182	0.12%	0.013%
21	15.522	2125	2131	2142	rBV	843637	1198580	64.19%	7.279%
22	15.657	2148	2154	2166	rBV	309207	433025	23.19%	2.630%
23	15.763	2169	2172	2175	rBV2	2550	2891	0.15%	0.018%
24	17.286	2425	2431	2437	rBV	621654	875458	46.89%	5.317%
25	17.386	2442	2448	2464	rVB	947216	1350466	72.33%	8.202%
26	18.180	2577	2583	2591	rBV3	7657	14067	0.75%	0.085%
27	19.251	2761	2765	2769	rBV3	10039	12748	0.68%	0.077%
28	19.322	2773	2777	2781	rBV	9929	12786	0.68%	0.078%
29	19.463	2798	2801	2807	rBV6	6921	11455	0.61%	0.070%
30	19.686	2833	2839	2848	rBV	1184716	1560242	83.56%	9.476%
31	21.486	3140	3145	3153	rBV	798768	1044678	55.95%	6.345%
32	23.739	3520	3528	3541	rBV3	864104	1867186	100.00%	11.340%
33	23.892	3547	3554	3564	rVB2	551287	1098793	58.85%	6.673%




Sum of corrected areas: 16465226

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022724.D
Acq On : 17 Nov 2022 17:41
Operator : CG/JU
Sample : PB149132BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK132

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

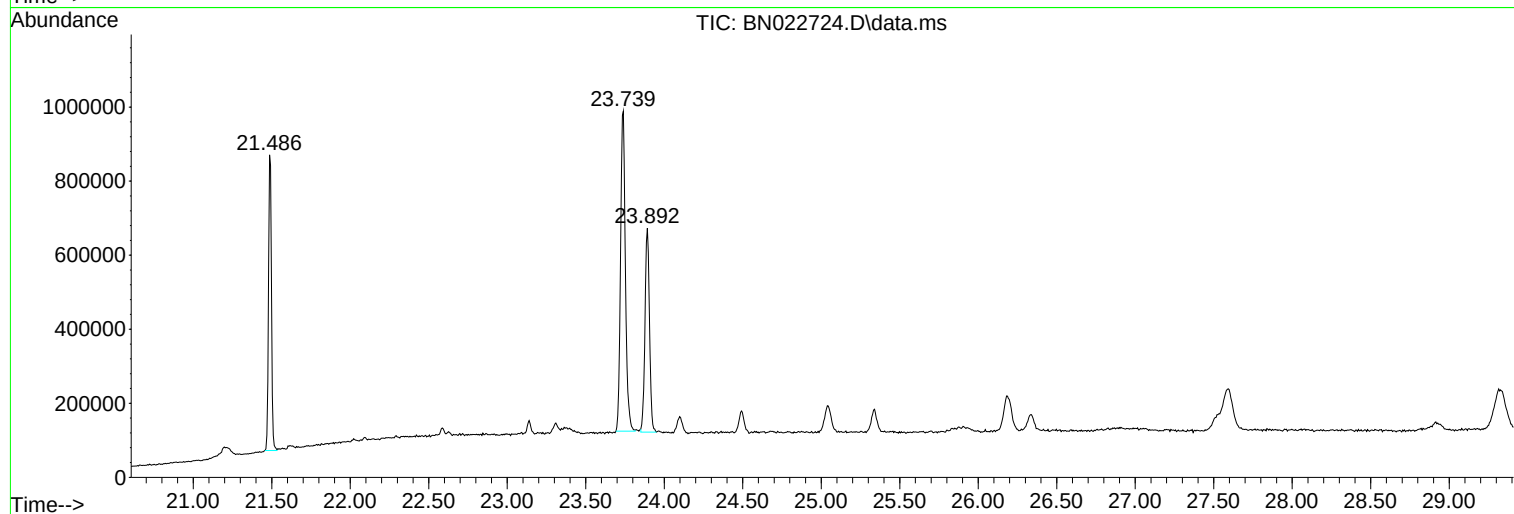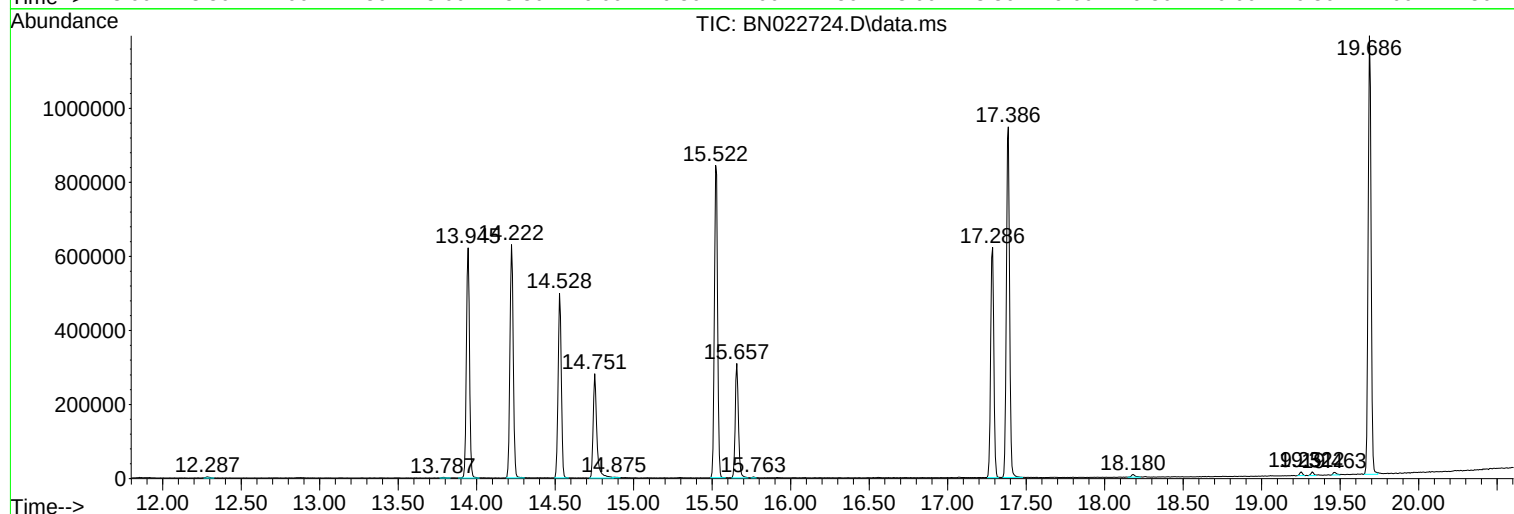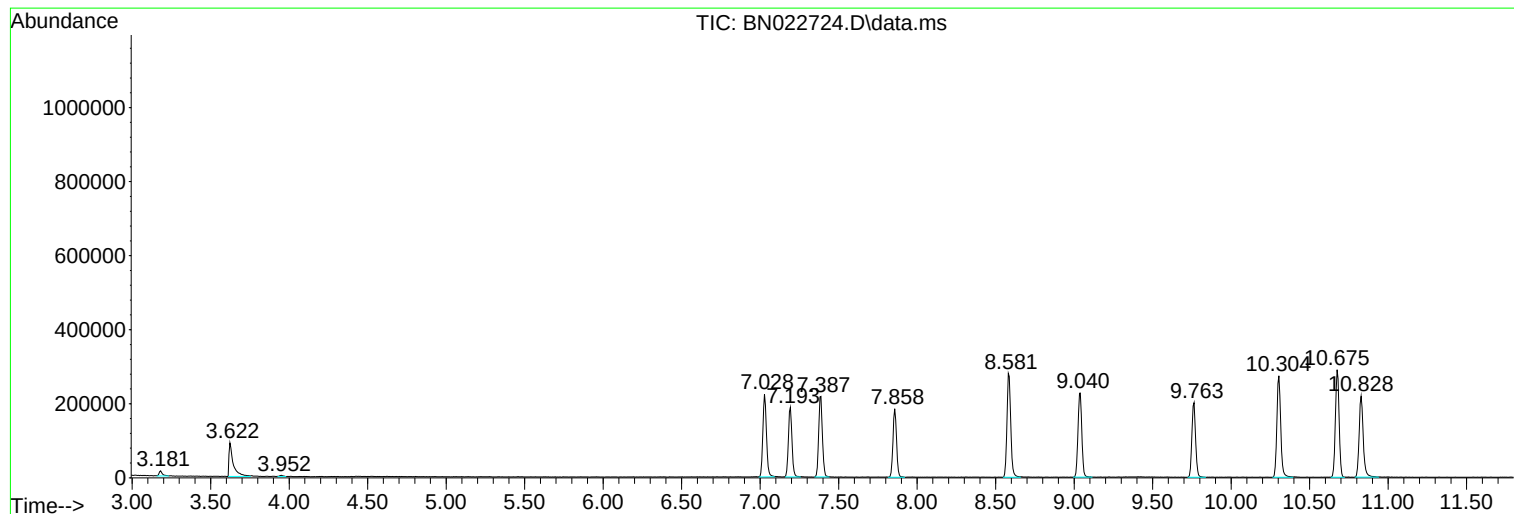

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022724.D
Acq On : 17 Nov 2022 17:41
Operator : CG/JU
Sample : PB149132BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK132

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022724.D
Acq On : 17 Nov 2022 17:41
Operator : CG/JU
Sample : PB149132BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK132

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc