

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022731.D
 Acq On : 17 Nov 2022 22:00
 Operator : CG/JU
 Sample : N5623-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	43	rVB	12071	17821	0.78%	0.095%
2	3.622	106	108	130	rBV	56882	113946	4.96%	0.605%
3	3.852	142	147	152	rVB2	5885	9888	0.43%	0.053%
4	3.946	159	163	169	rVB	3837	6014	0.26%	0.032%
5	7.028	682	687	695	rBV	64401	103250	4.49%	0.548%
6	7.187	708	714	729	rBV	221191	355444	15.47%	1.887%
7	7.381	741	747	758	rBV	209115	342454	14.91%	1.818%
8	7.857	821	828	841	rBV	205053	339313	14.77%	1.802%
9	7.963	842	846	849	rVB2	1981	2526	0.11%	0.013%
10	8.581	944	951	961	rBV	186489	304548	13.26%	1.617%
11	9.034	1021	1028	1041	rBV	293915	471383	20.52%	2.503%
12	9.757	1145	1151	1159	rBV	231815	379452	16.52%	2.015%
13	10.298	1237	1243	1257	rBV	302284	510899	22.24%	2.713%
14	10.675	1300	1307	1314	rBV	333680	548228	23.86%	2.911%
15	10.822	1325	1332	1350	rBV	307314	549217	23.91%	2.916%
16	11.351	1418	1422	1434	rVB3	2501	5680	0.25%	0.030%
17	11.904	1512	1516	1523	rVB4	1354	2709	0.12%	0.014%
18	12.286	1576	1581	1587	rVB	3495	6285	0.27%	0.033%
19	13.945	1853	1863	1872	rBV	712610	1016993	44.27%	5.400%
20	14.051	1876	1881	1885	rVB	12010	15233	0.66%	0.081%
21	14.222	1903	1910	1928	rBV	766430	1102081	47.97%	5.852%
22	14.527	1955	1962	1973	rBV	574768	833996	36.30%	4.428%
23	14.757	1995	2001	2013	rBV	55886	111918	4.87%	0.594%
24	14.963	2030	2036	2040	rVB5	5065	7018	0.31%	0.037%
25	15.521	2125	2131	2145	rVB	1065888	1461326	63.61%	7.759%
26	15.657	2148	2154	2166	rBV	372636	528304	22.99%	2.805%
27	15.763	2169	2172	2176	rVB3	3032	3787	0.16%	0.020%
28	16.410	2277	2282	2290	rVV3	1703	2854	0.12%	0.015%
29	17.280	2424	2430	2437	rBV	747127	1003417	43.67%	5.328%
30	17.380	2440	2447	2460	rVV	1269761	1773382	77.19%	9.416%
31	17.486	2462	2465	2469	rVB3	6609	7652	0.33%	0.041%
32	17.951	2538	2544	2548	rBV6	1087	2521	0.11%	0.013%
33	18.174	2578	2582	2588	rBV2	17835	26171	1.14%	0.139%
34	19.245	2760	2764	2771	rBV2	12230	17358	0.76%	0.092%
35	19.321	2773	2777	2782	rBV	11420	16272	0.71%	0.086%
36	19.457	2796	2800	2807	rBV2	17640	26123	1.14%	0.139%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022731.D
Acq On : 17 Nov 2022 22:00
Operator : CG/JU
Sample : N5623-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCB8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	19.686	2833	2839	2848	rBV	1530018	2020188	87.93%	10.727%
38	21.486	3140	3145	3152	rBV	918681	1153342	50.20%	6.124%
39	23.733	3519	3527	3538	rBV	1151318	2297474	100.00%	12.199%
40	23.886	3546	3553	3566	rVB2	596295	1219028	53.06%	6.473%
41	25.327	3794	3798	3807	rVB2	53044	117334	5.11%	0.623%




Sum of corrected areas: 18832829

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022731.D
Acq On : 17 Nov 2022 22:00
Operator : CG/JU
Sample : N5623-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

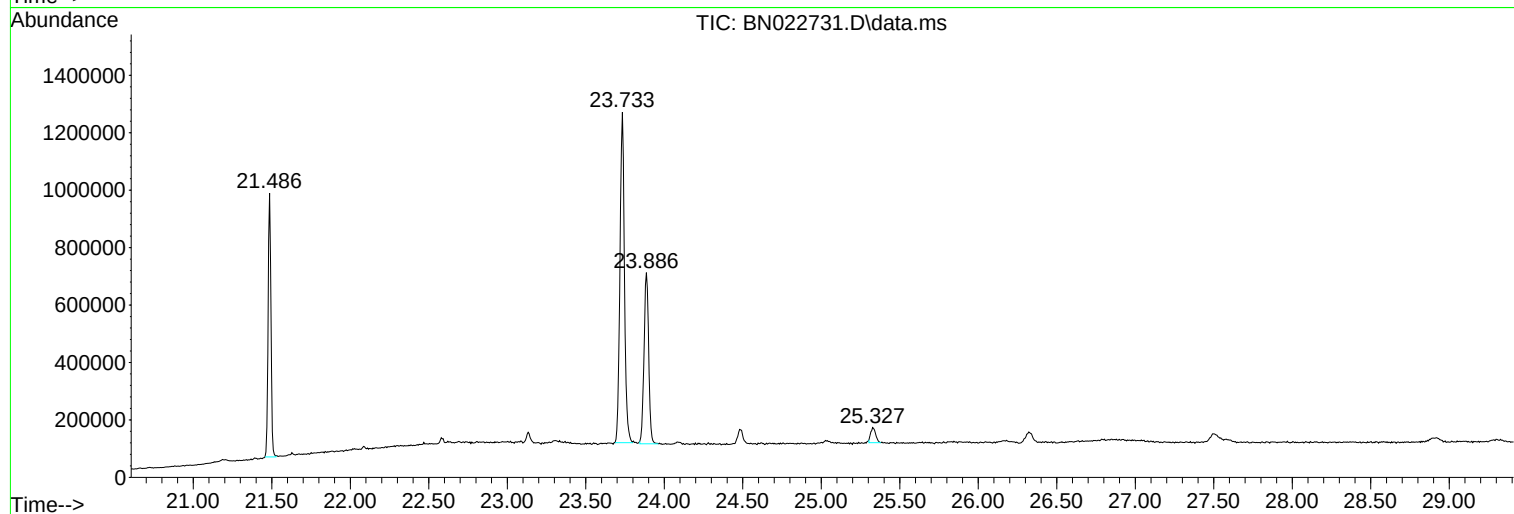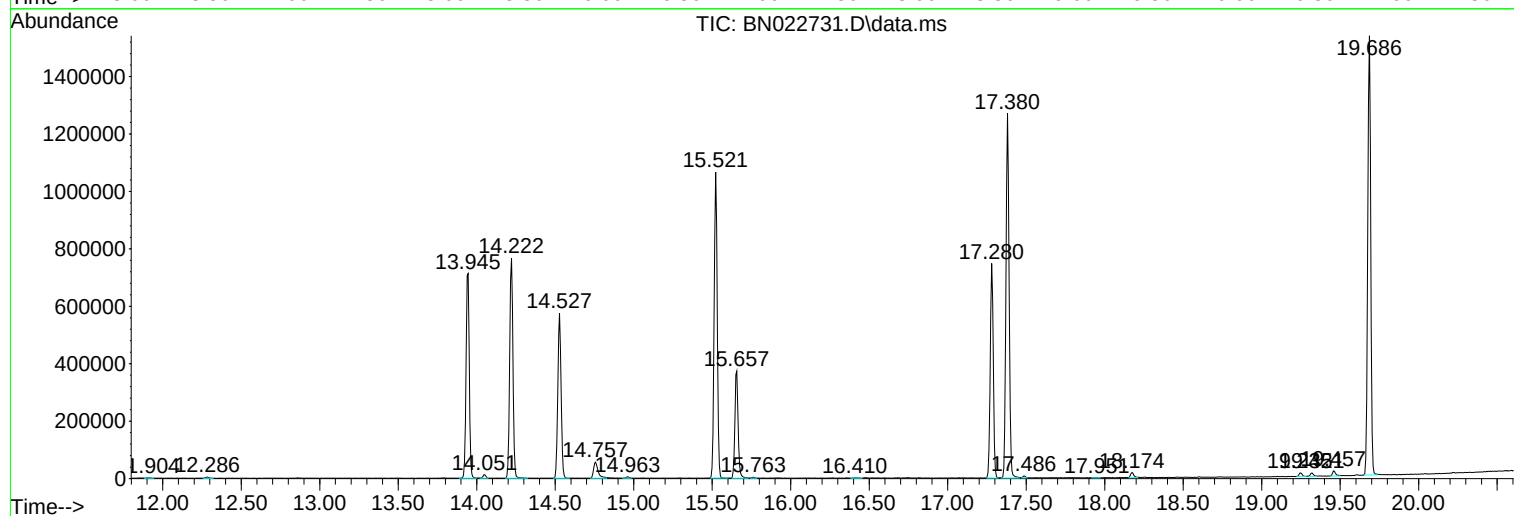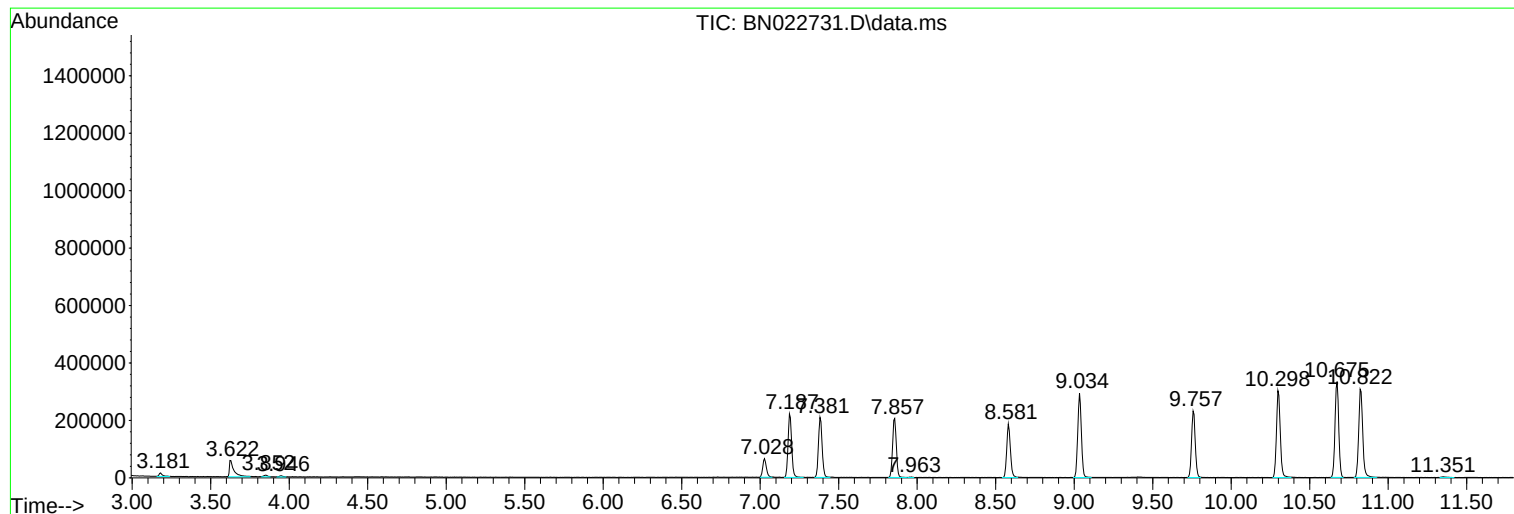

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022731.D
Acq On : 17 Nov 2022 22:00
Operator : CG/JU
Sample : N5623-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022731.D
Acq On : 17 Nov 2022 22:00
Operator : CG/JU
Sample : N5623-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc