

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022733.D
 Acq On : 17 Nov 2022 23:14
 Operator : CG/JU
 Sample : N5623-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	39	rBV	9681	13282	0.59%	0.080%
2	3.629	107	109	128	rBV	32989	65083	2.91%	0.393%
3	3.852	142	147	152	rVB2	5321	8939	0.40%	0.054%
4	3.952	159	164	170	rVB	3332	5371	0.24%	0.032%
5	4.364	233	234	244	rVB6	1240	2579	0.12%	0.016%
6	7.028	681	687	698	rVB	51562	86273	3.86%	0.521%
7	7.187	707	714	727	rBV	209170	326979	14.62%	1.975%
8	7.381	741	747	759	rBV	193340	304571	13.62%	1.839%
9	7.852	821	827	836	rBV	153334	249783	11.17%	1.509%
10	8.581	945	951	962	rBV	161023	262039	11.71%	1.583%
11	9.034	1021	1028	1038	rBV	266333	431117	19.27%	2.604%
12	9.152	1044	1048	1054	rVB5	1462	2791	0.12%	0.017%
13	9.758	1145	1151	1160	rBV	212194	342493	15.31%	2.068%
14	10.299	1236	1243	1260	rBV	269628	460036	20.57%	2.778%
15	10.675	1300	1307	1314	rVB	245120	407112	18.20%	2.459%
16	10.822	1326	1332	1349	rBV	217723	397212	17.76%	2.399%
17	12.287	1574	1581	1589	rVB2	3349	6232	0.28%	0.038%
18	13.416	1767	1773	1779	rVB	6687	9018	0.40%	0.054%
19	13.940	1856	1862	1874	rVB	690372	958869	42.87%	5.791%
20	14.222	1903	1910	1922	rBV	689378	1026356	45.88%	6.199%
21	14.528	1955	1962	1973	rVB	419726	610544	27.29%	3.687%
22	14.757	1995	2001	2013	rBV	48408	93761	4.19%	0.566%
23	14.963	2033	2036	2039	rBV2	3335	3339	0.15%	0.020%
24	15.522	2124	2131	2141	rBV	1016325	1398452	62.52%	8.446%
25	15.651	2147	2153	2166	rBV	373558	526728	23.55%	3.181%
26	15.763	2168	2172	2179	rVB	2903	3468	0.16%	0.021%
27	17.281	2424	2430	2436	rBV	564028	753129	33.67%	4.548%
28	17.381	2441	2447	2463	rVV	1251260	1744608	77.99%	10.536%
29	18.175	2578	2582	2588	rBV2	15162	21061	0.94%	0.127%
30	18.604	2650	2655	2659	rBV2	12946	14838	0.66%	0.090%
31	19.245	2760	2764	2769	rBV2	13616	18093	0.81%	0.109%
32	19.316	2771	2776	2782	rBV	11323	17197	0.77%	0.104%
33	19.363	2782	2784	2789	rVV5	1830	2869	0.13%	0.017%
34	19.457	2796	2800	2804	rBV	13860	18923	0.85%	0.114%
35	19.604	2822	2825	2828	rBV3	3311	4193	0.19%	0.025%
36	19.686	2832	2839	2851	rBV	1461123	1969751	88.06%	11.896%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022733.D
Acq On : 17 Nov 2022 23:14
Operator : CG/JU
Sample : N5623-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	21.486	3139	3145	3151	rBV	653785	859722	38.43%	5.192%
38	23.727	3519	3526	3540	rVB2	1087241	2236877	100.00%	13.509%
39	23.880	3546	3552	3563	rVB2	449462	894160	39.97%	5.400%




Sum of corrected areas: 16557848

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022733.D
Acq On : 17 Nov 2022 23:14
Operator : CG/JU
Sample : N5623-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

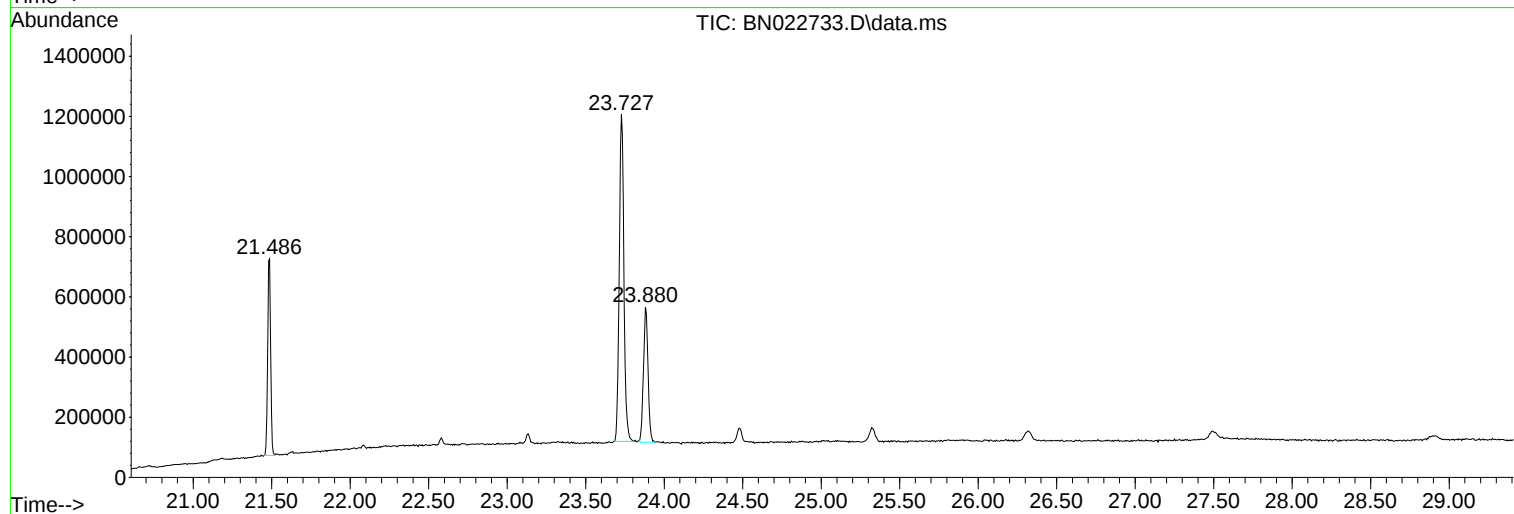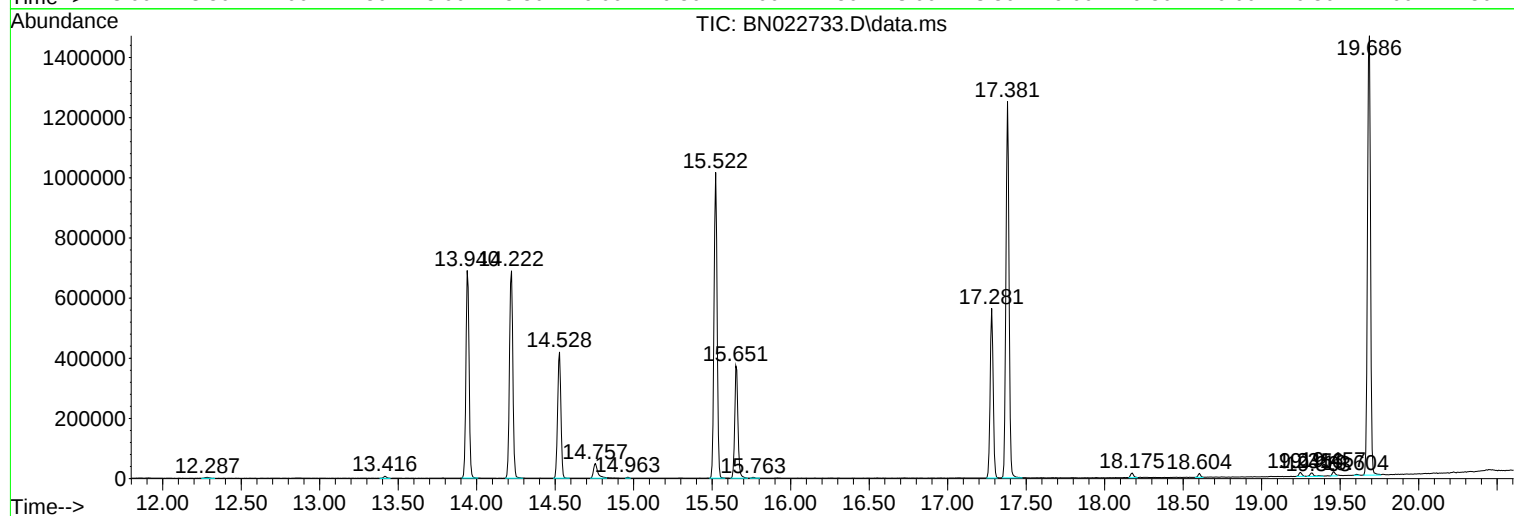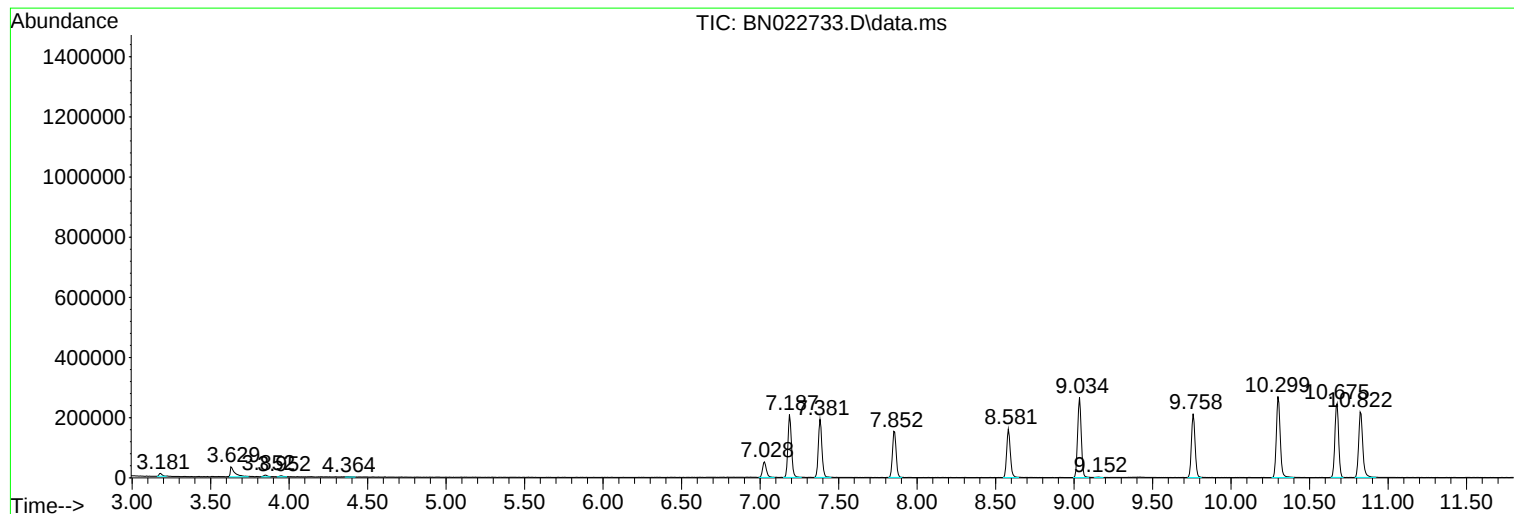

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022733.D
Acq On : 17 Nov 2022 23:14
Operator : CG/JU
Sample : N5623-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022733.D
Acq On : 17 Nov 2022 23:14
Operator : CG/JU
Sample : N5623-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc