

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022735.D
 Acq On : 18 Nov 2022 00:27
 Operator : CG/JU
 Sample : N5623-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	43	rVB	12744	20033	0.80%	0.098%
2	3.623	106	108	127	rBV	63489	122884	4.90%	0.602%
3	3.852	140	147	152	rBV	6249	11235	0.45%	0.055%
4	3.946	160	163	169	rVB	4253	5561	0.22%	0.027%
5	7.028	679	687	697	rBV	70016	116033	4.63%	0.568%
6	7.187	707	714	731	rBV	247593	386140	15.40%	1.892%
7	7.381	739	747	757	rBV	233269	374851	14.95%	1.836%
8	7.852	821	827	840	rVB	206670	340236	13.57%	1.667%
9	8.581	945	951	966	rBV	212905	340801	13.59%	1.670%
10	9.034	1020	1028	1043	rBV	322736	516039	20.58%	2.528%
11	9.169	1043	1051	1066	rBV	48454	91475	3.65%	0.448%
12	9.758	1144	1151	1162	rBV	267825	427469	17.05%	2.094%
13	10.299	1236	1243	1256	rBV	344534	575146	22.93%	2.818%
14	10.675	1299	1307	1316	rBV	325514	559340	22.30%	2.740%
15	10.822	1325	1332	1348	rBV	312296	561005	22.37%	2.748%
16	12.275	1573	1579	1586	rBV	4353	8048	0.32%	0.039%
17	12.422	1600	1604	1612	rBV3	5606	11397	0.45%	0.056%
18	13.416	1769	1773	1779	rVB2	2553	3650	0.15%	0.018%
19	13.940	1856	1862	1879	rVB	858466	1165877	46.49%	5.712%
20	14.222	1903	1910	1922	rBV	856871	1243794	49.60%	6.094%
21	14.528	1955	1962	1972	rBV	562709	850308	33.91%	4.166%
22	14.751	1995	2000	2019	rBV	70784	133520	5.32%	0.654%
23	14.963	2032	2036	2040	rVB5	3232	3730	0.15%	0.018%
24	15.522	2124	2131	2140	rBV	1192126	1641987	65.48%	8.044%
25	15.651	2148	2153	2167	rBV	446383	623957	24.88%	3.057%
26	15.763	2167	2172	2177	rBV3	3290	4535	0.18%	0.022%
27	17.281	2424	2430	2438	rBV	743720	1016763	40.54%	4.981%
28	17.381	2440	2447	2459	rBV2	1379127	1930171	76.97%	9.456%
29	18.175	2577	2582	2590	rBV2	22606	34116	1.36%	0.167%
30	18.604	2651	2655	2660	rVB4	2299	3621	0.14%	0.018%
31	19.245	2759	2764	2771	rBV2	15298	23146	0.92%	0.113%
32	19.316	2772	2776	2782	rVV	13212	18434	0.74%	0.090%
33	19.457	2796	2800	2808	rVB3	24734	34437	1.37%	0.169%
34	19.610	2822	2826	2829	rVB5	4169	4153	0.17%	0.020%
35	19.686	2833	2839	2853	rVV	1678213	2210976	88.16%	10.832%
36	21.486	3139	3145	3151	rBV	896211	1165403	46.47%	5.710%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022735.D
Acq On : 18 Nov 2022 00:27
Operator : CG/JU
Sample : N5623-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.733	3519	3527	3540	rVB2	1187724	2507776	100.00%	12.286%
38	23.886	3546	3553	3564	rVB2	607128	1215030	48.45%	5.953%
39	24.480	3651	3654	3662	rVB3	52679	108566	4.33%	0.532%




Sum of corrected areas: 20411643

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022735.D
Acq On : 18 Nov 2022 00:27
Operator : CG/JU
Sample : N5623-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

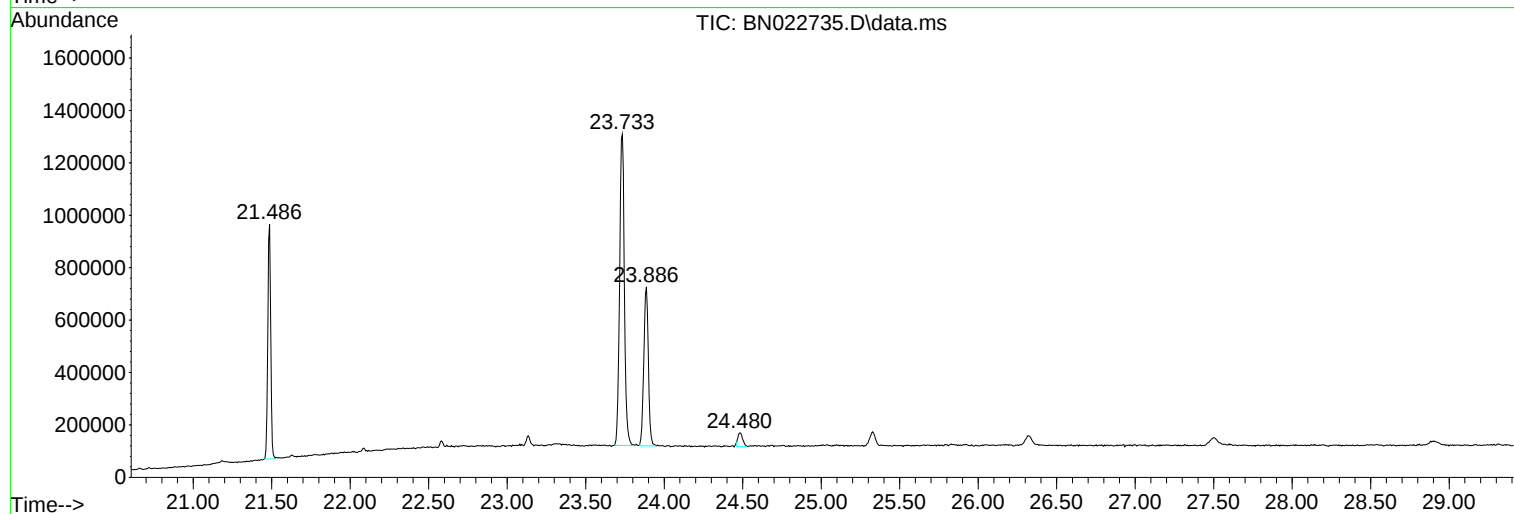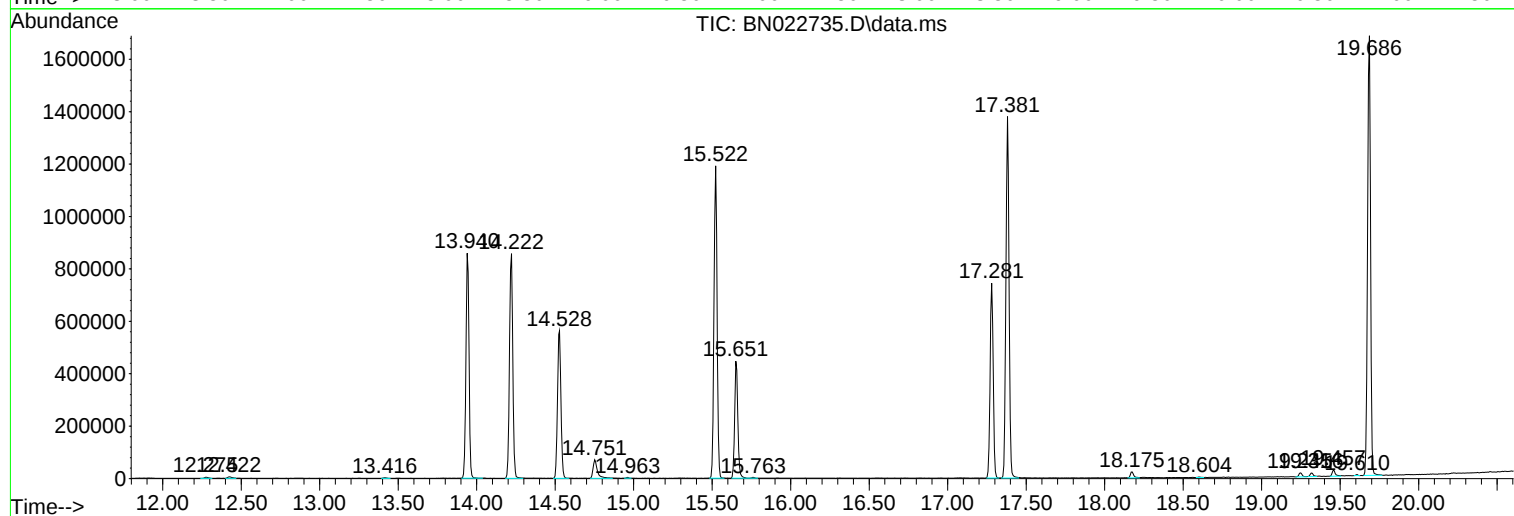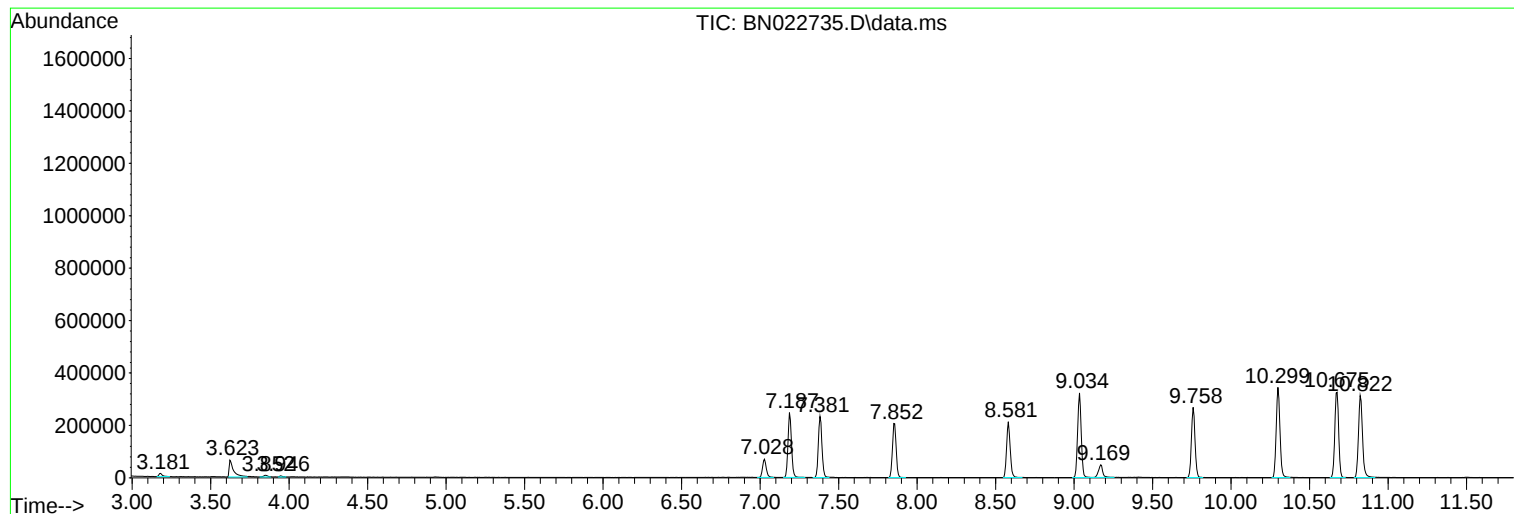

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022735.D
Acq On : 18 Nov 2022 00:27
Operator : CG/JU
Sample : N5623-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.169	5.38 ng/ul	91475	1,4-Dichlorobenzene-d4	7.858

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
2			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	83
4			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	72
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	72

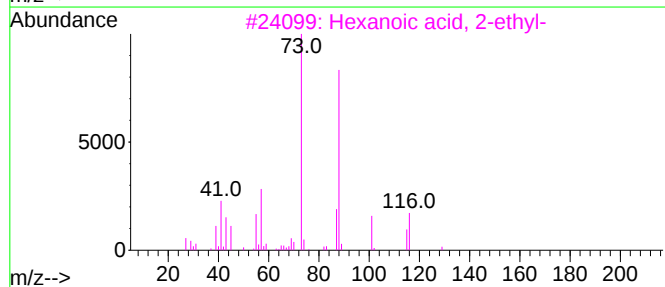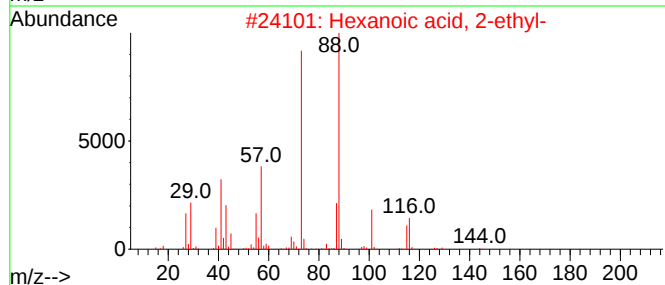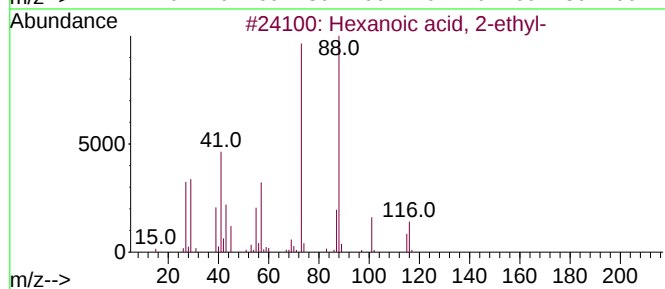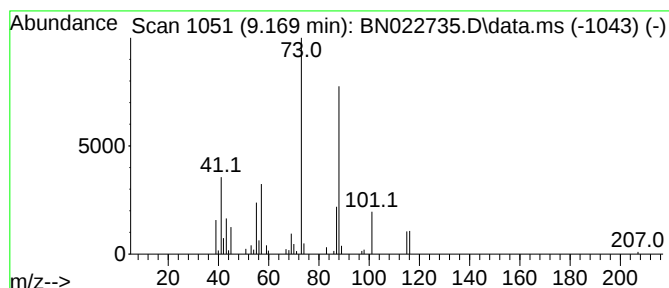

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022735.D
Acq On : 18 Nov 2022 00:27
Operator : CG/JU
Sample : N5623-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanoic acid, ...	9.169	5.4	ng/ul	91475	1	7.858	340236	20.0