

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022738.D
 Acq On : 18 Nov 2022 02:16
 Operator : CG/JU
 Sample : N5593-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	30	rBV	22043	31503	1.27%	0.154%
2	3.175	30	32	36	rVV	14860	19671	0.79%	0.096%
3	3.217	36	39	48	rVB	10289	15690	0.63%	0.077%
4	3.628	106	109	131	rBV	49165	99046	3.98%	0.484%
5	3.846	141	146	155	rVB	5768	10594	0.43%	0.052%
6	3.946	160	163	170	rVB	3510	5012	0.20%	0.025%
7	4.493	250	256	265	rBV	128092	203213	8.17%	0.993%
8	4.922	323	329	336	rBV	14823	23220	0.93%	0.114%
9	7.022	681	686	700	rBV	69105	116897	4.70%	0.571%
10	7.187	708	714	726	rBV	248003	392677	15.78%	1.920%
11	7.381	741	747	758	rBV	233774	375196	15.08%	1.834%
12	7.852	820	827	836	rBV	203743	329336	13.24%	1.610%
13	8.581	944	951	963	rBV	213090	345464	13.88%	1.689%
14	9.034	1020	1028	1043	rBV	323610	526820	21.17%	2.575%
15	9.410	1085	1092	1099	rVB4	1404	3370	0.14%	0.016%
16	9.757	1144	1151	1162	rBV	260206	419994	16.88%	2.053%
17	10.299	1236	1243	1259	rBV	339366	579077	23.27%	2.831%
18	10.669	1300	1306	1314	rBV	326428	548225	22.03%	2.680%
19	10.822	1325	1332	1351	rBV	300163	537971	21.62%	2.630%
20	12.275	1575	1579	1587	rBV2	4036	7053	0.28%	0.034%
21	13.940	1856	1862	1879	rVB	827743	1143895	45.97%	5.592%
22	14.216	1903	1909	1923	rBV	843639	1242094	49.92%	6.072%
23	14.528	1955	1962	1971	rBV	543553	809144	32.52%	3.955%
24	14.751	1993	2000	2023	rBV	68766	135487	5.44%	0.662%
25	15.522	2124	2131	2143	rVB	1164090	1597062	64.18%	7.807%
26	15.651	2148	2153	2167	rVB	453407	608374	24.45%	2.974%
27	15.763	2167	2172	2176	rVB	3039	3880	0.16%	0.019%
28	17.075	2389	2395	2399	rBV5	3132	5474	0.22%	0.027%
29	17.281	2424	2430	2437	rBV	726218	1005263	40.40%	4.914%
30	17.381	2440	2447	2462	rBV	1321797	1878324	75.49%	9.182%
31	17.686	2491	2499	2503	rBV9	2721	6255	0.25%	0.031%
32	17.951	2540	2544	2548	rBV3	9671	11276	0.45%	0.055%
33	18.175	2576	2582	2587	rBV2	42357	61507	2.47%	0.301%
34	18.416	2620	2623	2628	rBV7	2589	3877	0.16%	0.019%
35	18.786	2684	2686	2691	rBV5	2759	4422	0.18%	0.022%
36	19.245	2760	2764	2771	rBV4	18530	33378	1.34%	0.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022738.D
 Acq On : 18 Nov 2022 02:16
 Operator : CG/JU
 Sample : N5593-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	19.316	2772	2776	2783	rBV2	17015	27708	1.11%	0.135%
38	19.457	2796	2800	2807	rBV2	34790	52275	2.10%	0.256%
39	19.604	2823	2825	2829	rBV5	7380	7179	0.29%	0.035%
40	19.686	2832	2839	2844	rBV	1580719	2168687	87.16%	10.601%
41	21.486	3139	3145	3154	rBV	894355	1174131	47.19%	5.740%
42	22.721	3351	3355	3361	rVB	58579	81762	3.29%	0.400%
43	23.727	3519	3526	3542	rVB2	1198441	2488289	100.00%	12.164%
44	23.886	3546	3553	3562	rVB2	603248	1201339	48.28%	5.873%
45	24.480	3651	3654	3661	rVB	63594	115543	4.64%	0.565%


Sum of corrected areas: 20456654

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022738.D
Acq On : 18 Nov 2022 02:16
Operator : CG/JU
Sample : N5593-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

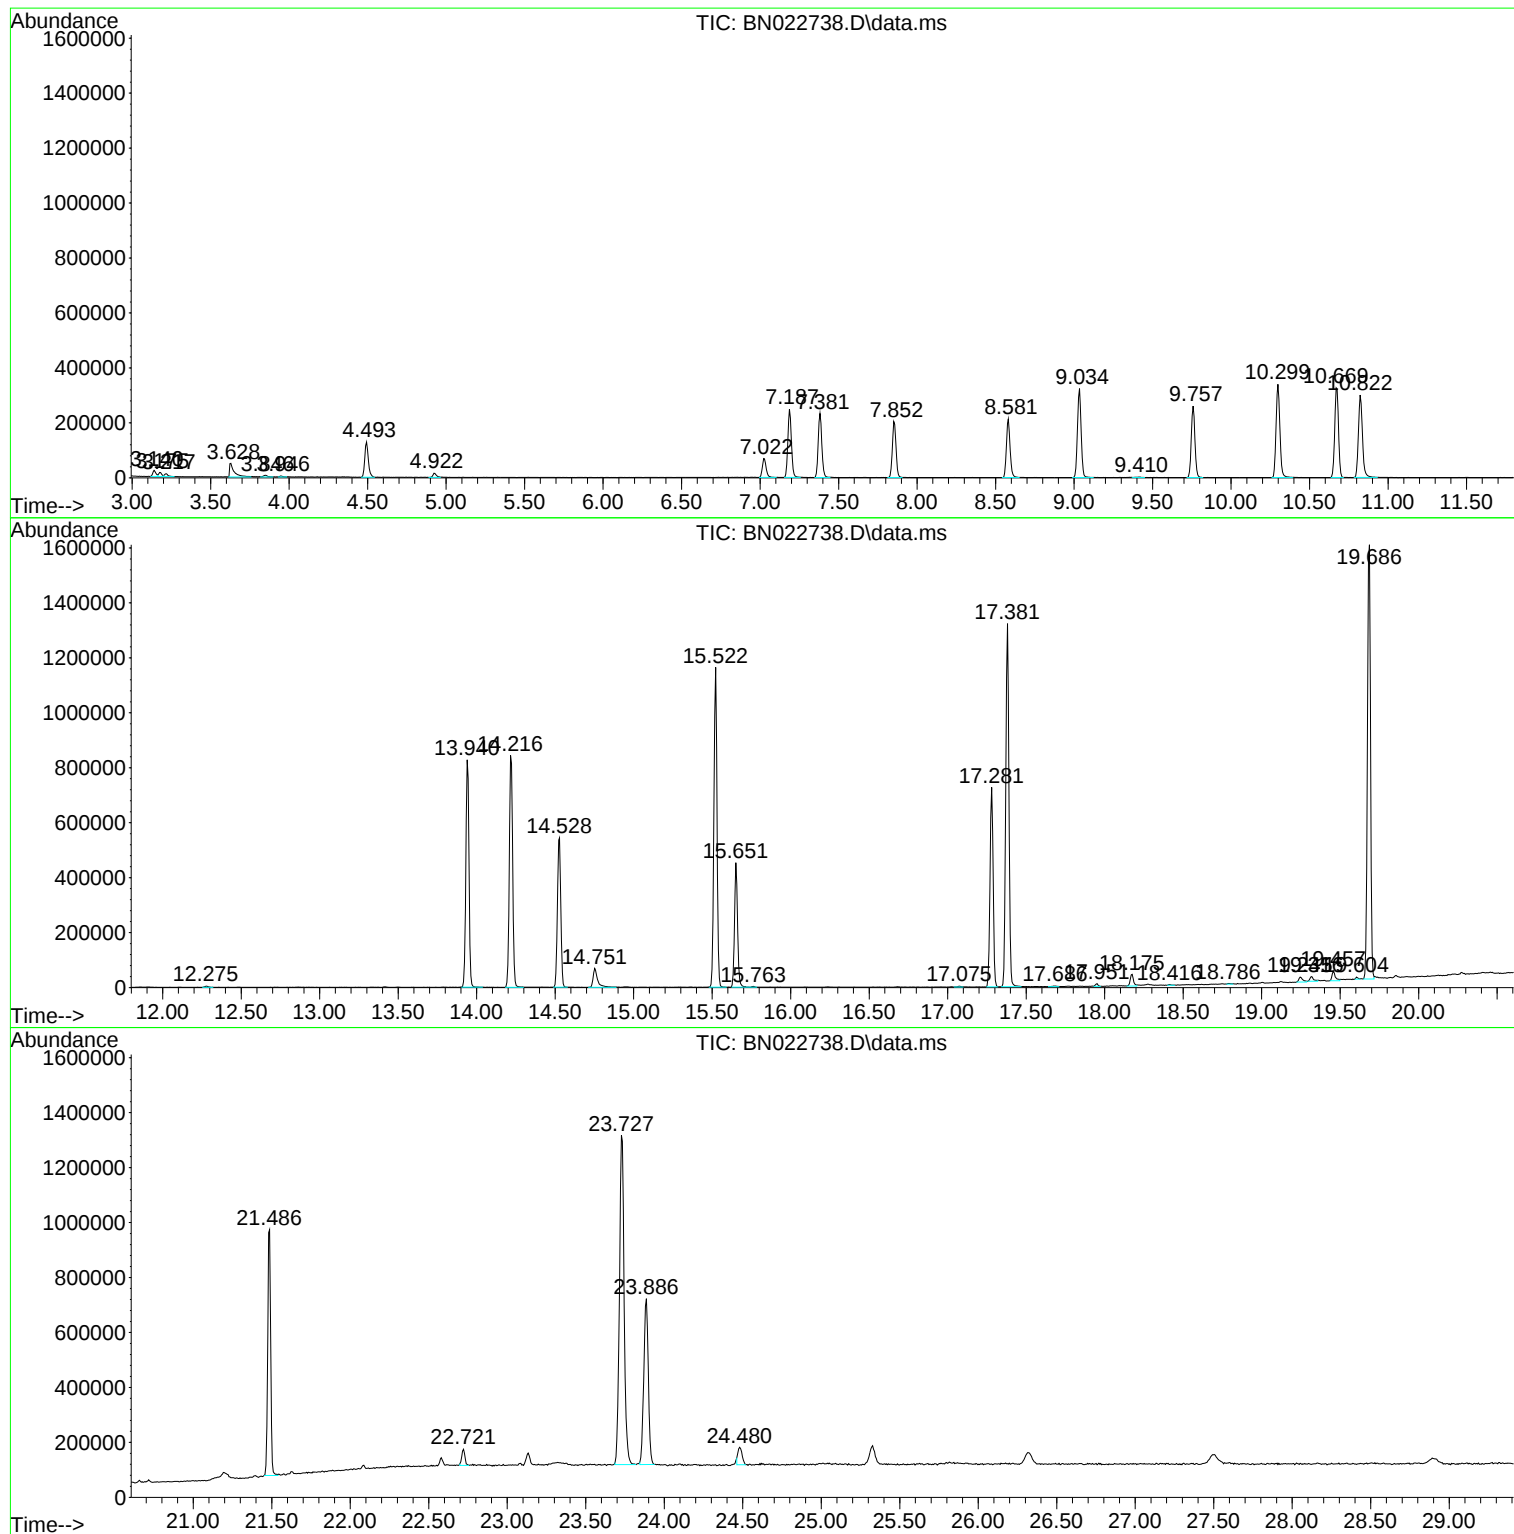

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022738.D
Acq On : 18 Nov 2022 02:16
Operator : CG/JU
Sample : N5593-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022738.D
Acq On : 18 Nov 2022 02:16
Operator : CG/JU
Sample : N5593-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AE2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc