

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022742.D
 Acq On : 18 Nov 2022 05:18
 Operator : CG/JU
 Sample : PB149055BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rBV	17324	25043	1.14%	0.122%
2	3.617	104	107	126	rBV	221230	396227	18.02%	1.937%
3	3.946	159	163	169	rVB2	3292	5615	0.26%	0.027%
4	7.022	680	686	703	rVB	300438	484362	22.03%	2.368%
5	7.187	708	714	726	rVB	249583	392121	17.84%	1.917%
6	7.381	740	747	758	rBV	297812	475727	21.64%	2.326%
7	7.852	821	827	838	rBV	189484	304219	13.84%	1.487%
8	8.581	944	951	966	rBV	374065	630301	28.67%	3.081%
9	9.034	1020	1028	1041	rBV	311597	520836	23.69%	2.546%
10	9.757	1144	1151	1160	rBV	274750	447235	20.34%	2.186%
11	10.299	1236	1243	1253	rBV	367502	631839	28.74%	3.089%
12	10.669	1299	1306	1313	rBV	298374	500054	22.75%	2.445%
13	10.822	1324	1332	1350	rBV	410741	721529	32.82%	3.527%
14	12.281	1576	1580	1587	rVB2	3983	7485	0.34%	0.037%
15	13.940	1853	1862	1874	rBV	836516	1152894	52.45%	5.636%
16	14.216	1902	1909	1924	rBV	853011	1235578	56.21%	6.040%
17	14.522	1955	1961	1972	rVB	505242	734883	33.43%	3.593%
18	14.745	1993	1999	2017	rBV	399007	620024	28.20%	3.031%
19	15.522	2124	2131	2146	rBV	1078789	1575834	71.68%	7.704%
20	15.651	2148	2153	2167	rBV	431640	584548	26.59%	2.858%
21	15.763	2167	2172	2175	rVB	3666	4428	0.20%	0.022%
22	17.281	2423	2430	2438	rBV	659182	896827	40.80%	4.384%
23	17.381	2440	2447	2458	rBV	1222245	1772546	80.63%	8.665%
24	19.245	2760	2764	2769	rBV3	12896	17591	0.80%	0.086%
25	19.316	2772	2776	2780	rBV2	11284	15831	0.72%	0.077%
26	19.686	2832	2839	2850	rBV	1475831	2024224	92.08%	9.896%
27	21.480	3139	3144	3153	rBV	789011	1037308	47.19%	5.071%
28	23.727	3518	3526	3540	rBV2	1161058	2198281	100.00%	10.747%
29	23.880	3545	3552	3562	rVB2	530766	1042017	47.40%	5.094%


Sum of corrected areas: 20455407

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022742.D
Acq On : 18 Nov 2022 05:18
Operator : CG/JU
Sample : PB149055BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

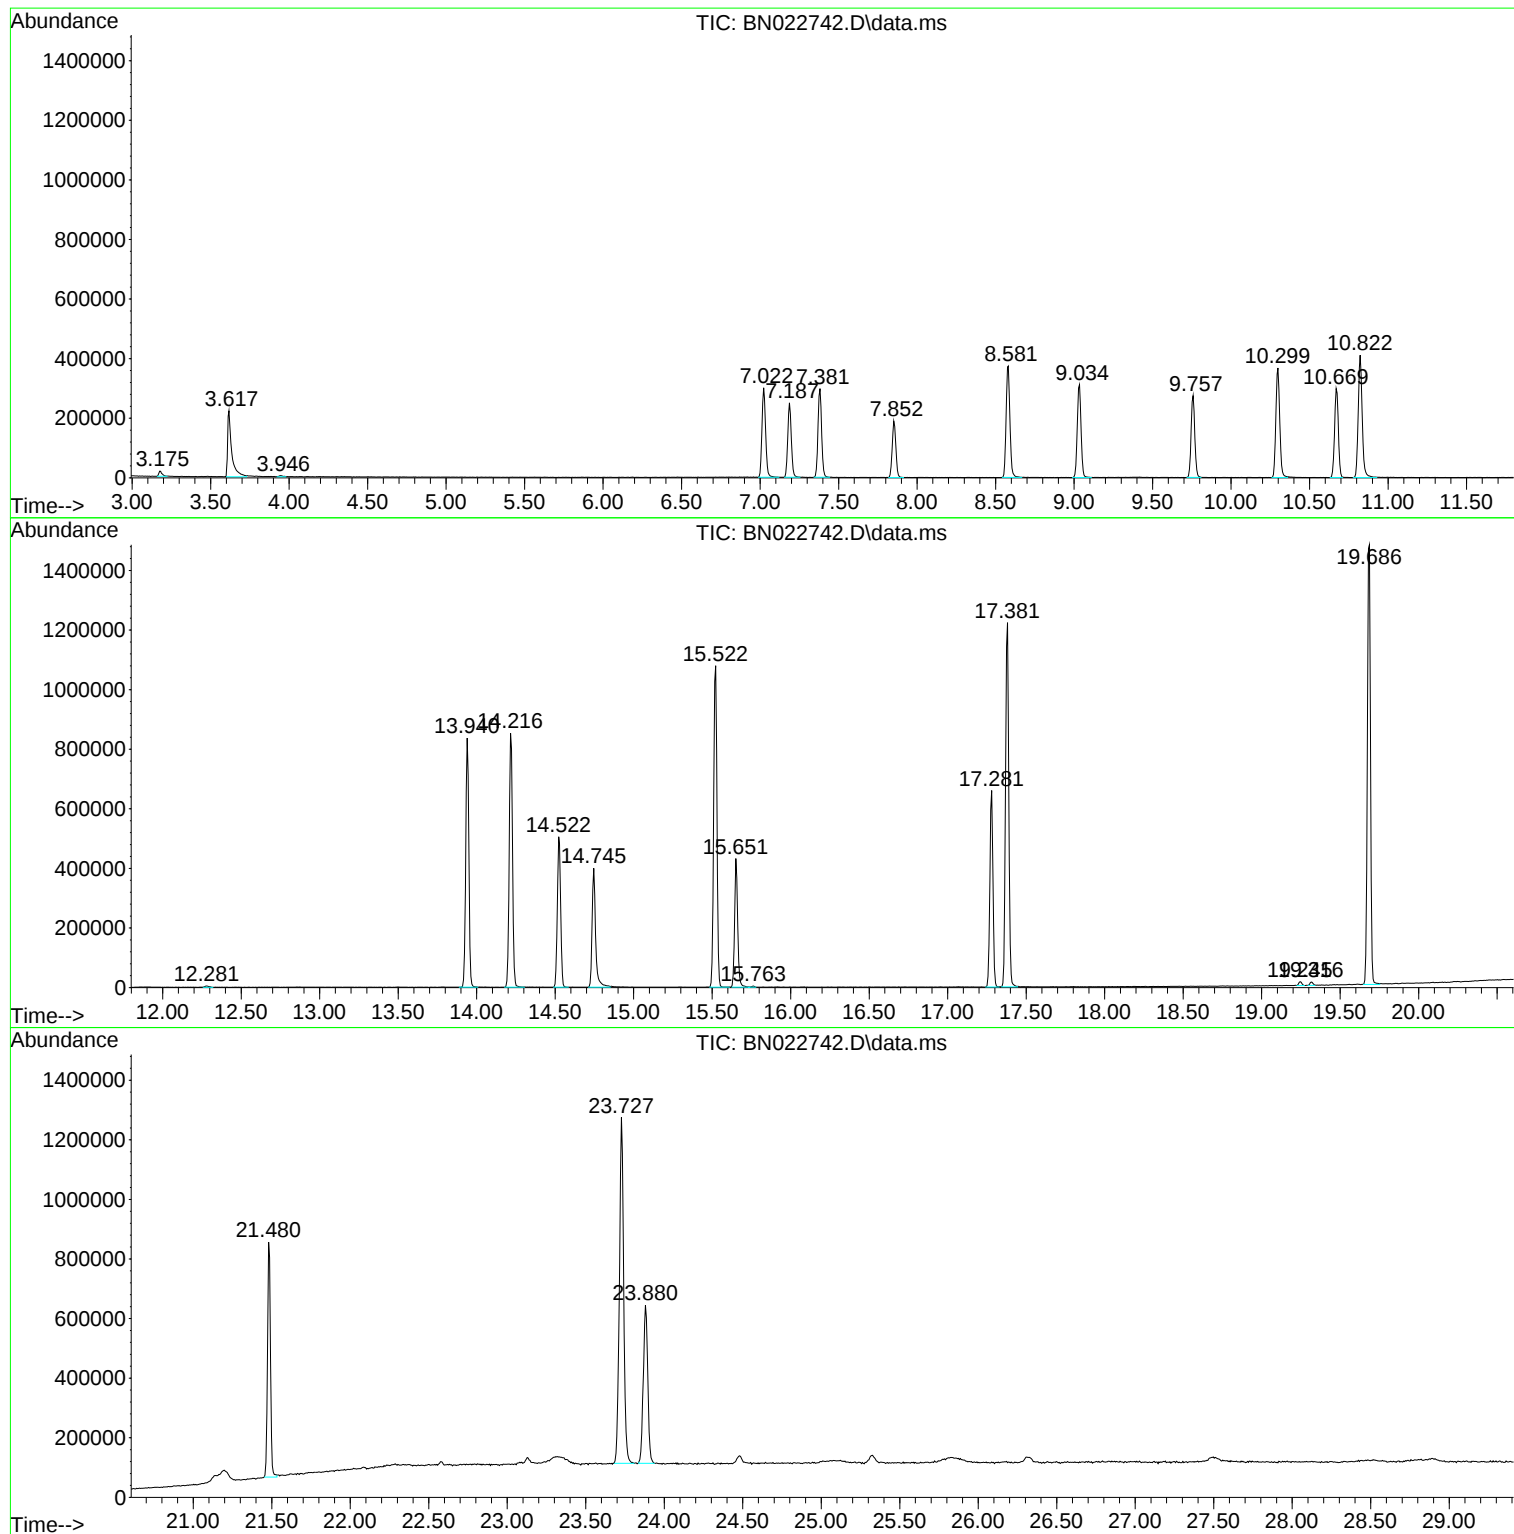

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022742.D
Acq On : 18 Nov 2022 05:18
Operator : CG/JU
Sample : PB149055BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022742.D
Acq On : 18 Nov 2022 05:18
Operator : CG/JU
Sample : PB149055BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc