

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022746.D
 Acq On : 18 Nov 2022 08:31
 Operator : CG/JU
 Sample : PB149074BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK074

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	42	rVB	17385	26275	1.29%	0.136%
2	3.611	103	106	124	rBV	197083	345257	16.96%	1.784%
3	3.946	159	163	170	rVB3	4308	7778	0.38%	0.040%
4	6.958	670	675	679	rVB4	1196	2249	0.11%	0.012%
5	7.016	679	685	700	rBV	282598	444734	21.85%	2.298%
6	7.181	707	713	727	rBV	229990	360797	17.72%	1.865%
7	7.375	739	746	759	rBV	271570	435621	21.40%	2.251%
8	7.846	819	826	836	rBV	211800	342592	16.83%	1.771%
9	8.575	943	950	962	rBV	348945	570380	28.02%	2.948%
10	9.028	1020	1027	1041	rBV	290884	471650	23.17%	2.438%
11	9.752	1144	1150	1159	rBV	246024	401719	19.73%	2.076%
12	10.293	1234	1242	1258	rBV	336281	574240	28.21%	2.968%
13	10.669	1297	1306	1314	rBV	330224	557438	27.38%	2.881%
14	10.816	1324	1331	1346	rBV	360117	636229	31.25%	3.288%
15	11.834	1496	1504	1506	rBV5	1612	3473	0.17%	0.018%
16	12.281	1575	1580	1586	rBV3	3585	6596	0.32%	0.034%
17	12.857	1669	1678	1681	rBV3	1786	4242	0.21%	0.022%
18	13.781	1829	1835	1840	rBV4	1682	3127	0.15%	0.016%
19	13.940	1849	1862	1872	rBV	745143	1024035	50.30%	5.292%
20	14.216	1902	1909	1923	rBV2	767039	1112162	54.63%	5.748%
21	14.522	1955	1961	1968	rBV	574799	811361	39.85%	4.193%
22	14.745	1993	1999	2022	rBV	329990	541740	26.61%	2.800%
23	15.292	2088	2092	2097	rVB2	1498	2311	0.11%	0.012%
24	15.516	2124	2130	2138	rVV	983327	1426697	70.08%	7.373%
25	15.651	2147	2153	2166	rBV	364600	501989	24.66%	2.594%
26	15.757	2166	2171	2175	rVB4	3080	4815	0.24%	0.025%
27	16.551	2302	2306	2313	rBV6	1490	2738	0.13%	0.014%
28	17.281	2423	2430	2438	rBV	693520	982617	48.27%	5.078%
29	17.381	2440	2447	2459	rBV2	1097861	1591898	78.19%	8.227%
30	19.245	2760	2764	2769	rVB2	10033	13325	0.65%	0.069%
31	19.322	2772	2777	2781	rBV	9861	13204	0.65%	0.068%
32	19.686	2833	2839	2851	rBV	1313972	1801568	88.49%	9.311%
33	21.486	3140	3145	3157	rBV	893027	1141146	56.05%	5.898%
34	23.733	3519	3527	3540	rVB2	980565	2035817	100.00%	10.521%
35	23.886	3546	3553	3563	rVB	587206	1147745	56.38%	5.932%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022746.D
Acq On : 18 Nov 2022 08:31
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK074

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 19349565

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022746.D
Acq On : 18 Nov 2022 08:31
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

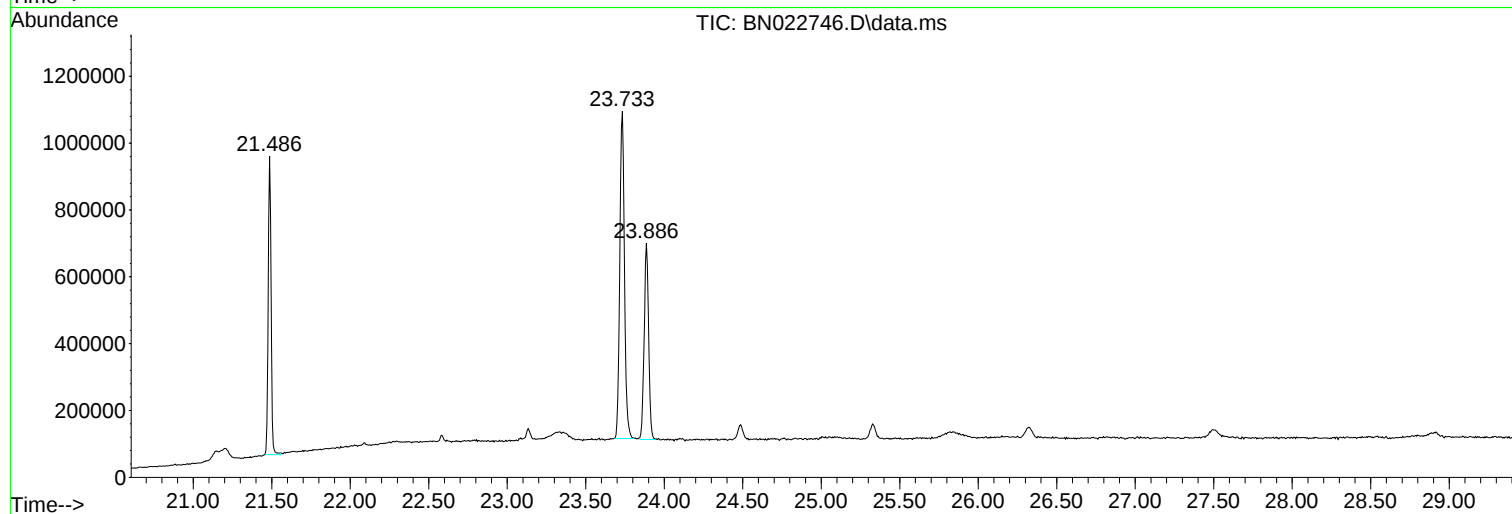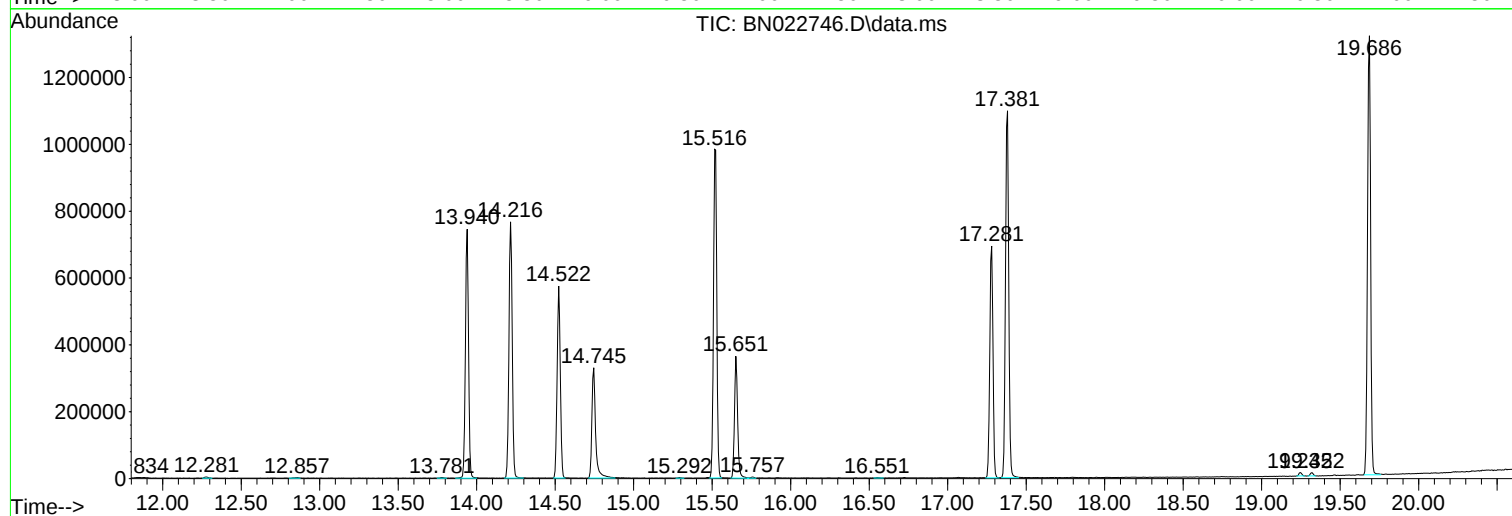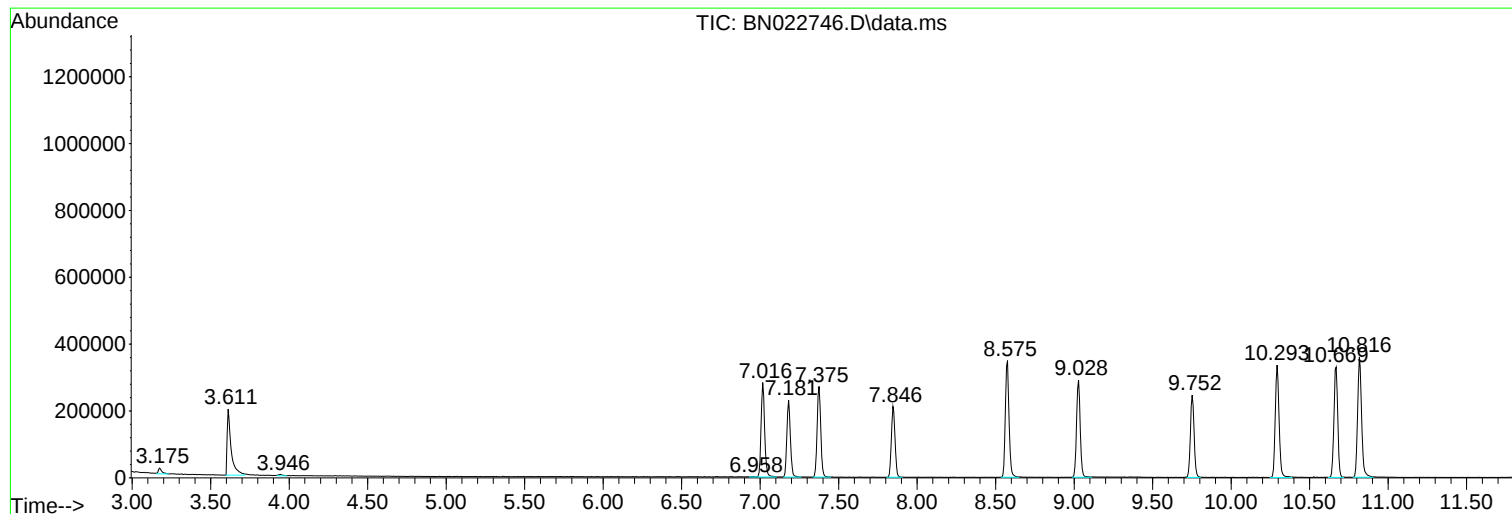

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022746.D
Acq On : 18 Nov 2022 08:31
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022746.D
Acq On : 18 Nov 2022 08:31
Operator : CG/JU
Sample : PB149074BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK074

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc