

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022749.D
 Acq On : 18 Nov 2022 10:20
 Operator : CG/JU
 Sample : PB149146BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	44	rVB	13497	21934	1.18%	0.122%
2	3.616	103	107	132	rBV	172120	309688	16.63%	1.718%
3	3.946	158	163	168	rBV3	3885	5606	0.30%	0.031%
4	7.022	680	686	700	rBV	239335	388836	20.88%	2.157%
5	7.187	707	714	728	rBV	202612	316966	17.02%	1.758%
6	7.381	740	747	757	rBV	236570	382333	20.53%	2.121%
7	7.852	820	827	838	rBV	207646	335754	18.03%	1.863%
8	8.575	944	950	962	rBV	299346	503311	27.03%	2.792%
9	9.034	1021	1028	1038	rBV	250896	417359	22.41%	2.315%
10	9.757	1144	1151	1161	rBV	222158	357618	19.20%	1.984%
11	10.298	1236	1243	1255	rBV	291134	506332	27.19%	2.809%
12	10.669	1299	1306	1314	rBV	333458	554642	29.78%	3.077%
13	10.822	1323	1332	1349	rBV	322847	577122	30.99%	3.202%
14	12.281	1576	1580	1586	rVB	3605	6012	0.32%	0.033%
15	13.939	1856	1862	1873	rVB	688473	921877	49.50%	5.114%
16	14.216	1903	1909	1922	rBV2	694130	997251	53.55%	5.532%
17	14.522	1955	1961	1971	rVB	560964	816467	43.84%	4.529%
18	14.745	1993	1999	2021	rBV	299255	495413	26.60%	2.748%
19	15.522	2124	2131	2141	rVB	898827	1285914	69.05%	7.133%
20	15.651	2147	2153	2167	rBV	330697	461772	24.80%	2.562%
21	15.757	2169	2171	2176	rVB2	3046	3117	0.17%	0.017%
22	17.075	2390	2395	2398	rBV5	1595	2872	0.15%	0.016%
23	17.280	2423	2430	2437	rBV	705515	999780	53.69%	5.546%
24	17.380	2440	2447	2460	rVV	1001271	1466959	78.77%	8.138%
25	19.245	2760	2764	2769	rBV	10854	14681	0.79%	0.081%
26	19.316	2772	2776	2781	rVB2	11224	14354	0.77%	0.080%
27	19.680	2832	2838	2849	rVV	1221704	1679780	90.20%	9.318%
28	21.486	3139	3145	3151	rBV2	867993	1143840	61.42%	6.345%
29	23.727	3519	3526	3540	rVB2	920866	1862299	100.00%	10.331%
30	23.880	3545	3552	3563	rVB2	567075	1176671	63.18%	6.527%




Sum of corrected areas: 18026560

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022749.D
Acq On : 18 Nov 2022 10:20
Operator : CG/JU
Sample : PB149146BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

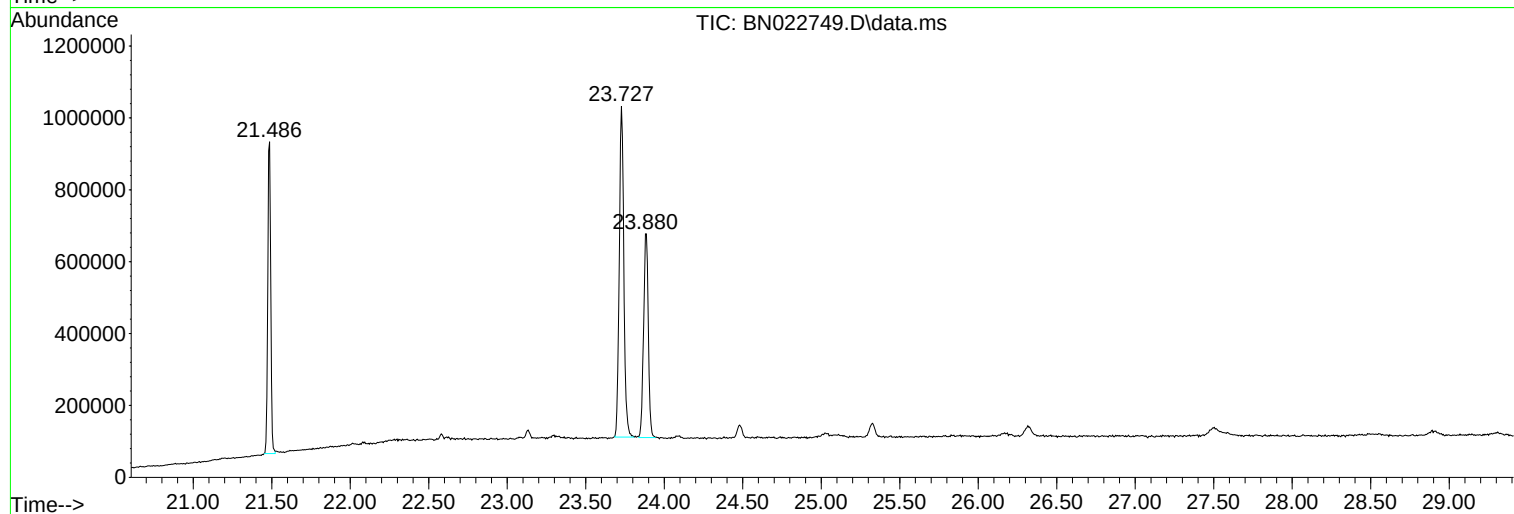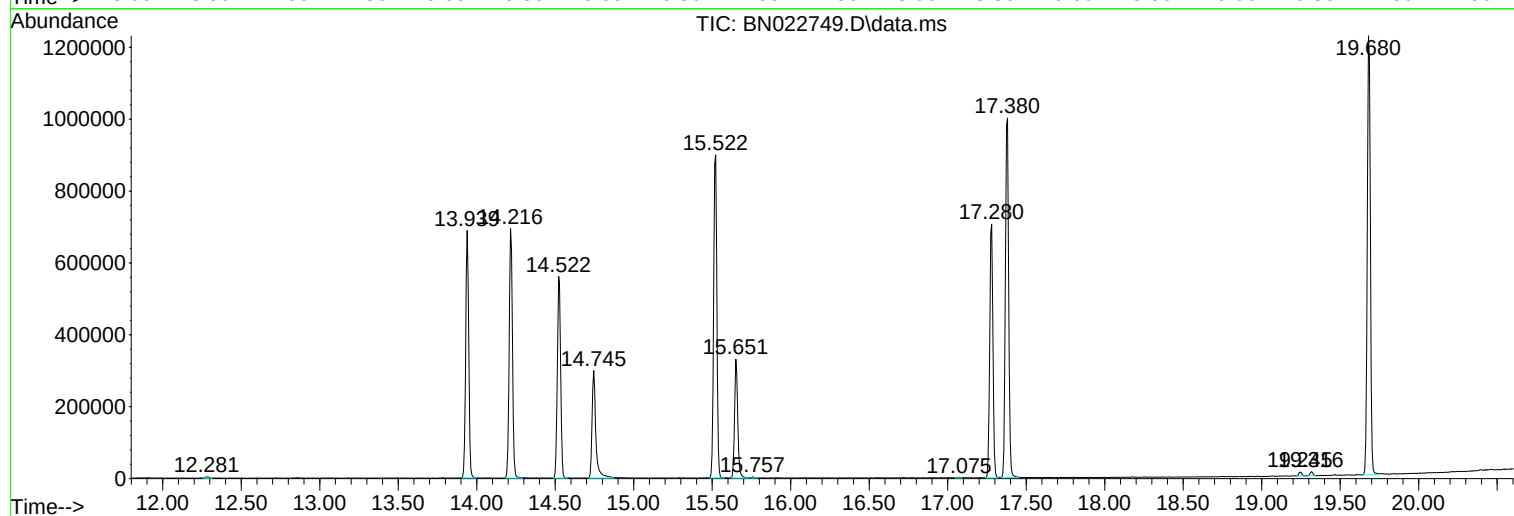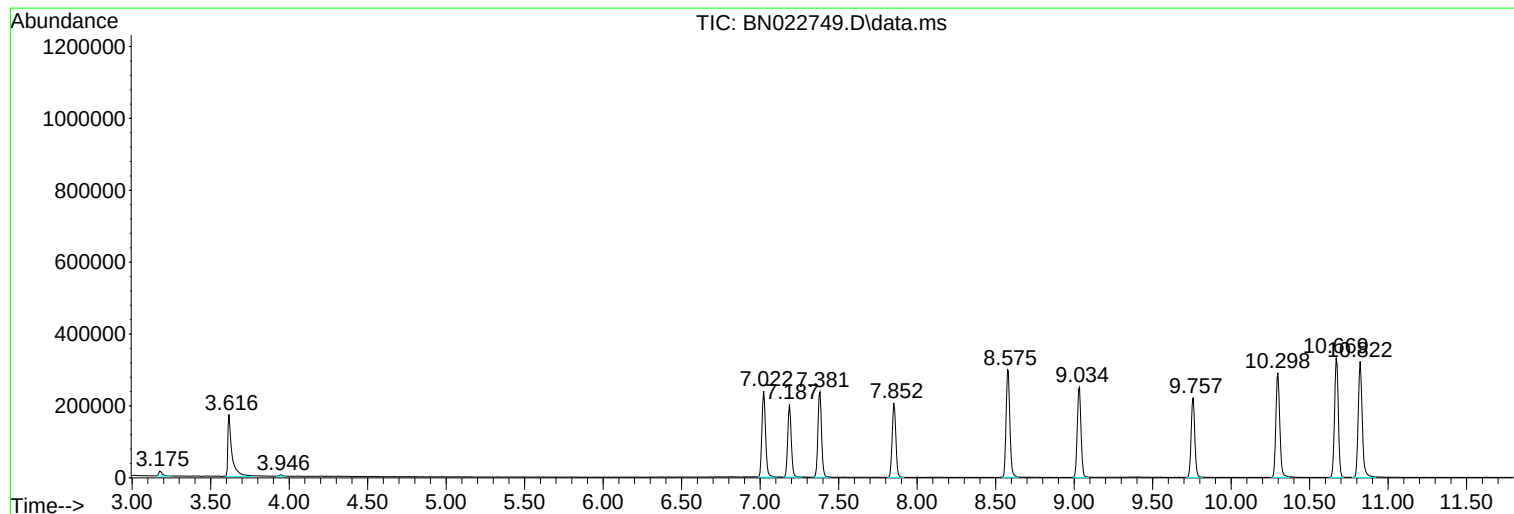

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022749.D
Acq On : 18 Nov 2022 10:20
Operator : CG/JU
Sample : PB149146BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022749.D
Acq On : 18 Nov 2022 10:20
Operator : CG/JU
Sample : PB149146BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK146

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc