

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022754.D
 Acq On : 18 Nov 2022 13:23
 Operator : CG/JU
 Sample : N5689-02
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rBV	10429	13759	0.62%	0.076%
2	3.481	81	84	98	rBV	11655	22289	1.00%	0.122%
3	3.628	107	109	125	rBV	38499	73994	3.34%	0.406%
4	3.846	141	146	152	rVB2	6971	11410	0.51%	0.063%
5	3.946	159	163	170	rBV2	3591	5851	0.26%	0.032%
6	7.022	681	686	693	rBV	50221	79635	3.59%	0.437%
7	7.187	708	714	725	rBV	233594	366970	16.55%	2.015%
8	7.381	740	747	755	rBV	203513	334784	15.09%	1.838%
9	7.852	821	827	839	rVB	198794	318350	14.35%	1.748%
10	8.575	945	950	962	rBV	160182	267100	12.04%	1.467%
11	9.034	1020	1028	1036	rBV	288117	487646	21.99%	2.678%
12	9.757	1144	1151	1159	rBV	236464	388118	17.50%	2.131%
13	10.299	1236	1243	1257	rBV	300324	522556	23.56%	2.869%
14	10.669	1299	1306	1315	rVB	313862	519202	23.41%	2.851%
15	10.822	1323	1332	1346	rBV	264871	486871	21.95%	2.673%
16	11.910	1512	1517	1521	rVB2	1210	2359	0.11%	0.013%
17	12.281	1574	1580	1586	rBV3	4066	7761	0.35%	0.043%
18	13.940	1856	1862	1872	rVB	765223	1044402	47.09%	5.735%
19	14.216	1902	1909	1920	rBV	814509	1154463	52.05%	6.339%
20	14.522	1955	1961	1970	rBV	540588	774083	34.90%	4.250%
21	14.751	1995	2000	2019	rBV	40071	81430	3.67%	0.447%
22	14.957	2032	2035	2041	rVB3	5917	7815	0.35%	0.043%
23	15.522	2124	2131	2139	rBV	1073043	1516239	68.36%	8.325%
24	15.651	2148	2153	2167	rBV	362460	491901	22.18%	2.701%
25	15.757	2167	2171	2176	rVB4	2866	4360	0.20%	0.024%
26	17.281	2423	2430	2437	rBV	665023	949587	42.81%	5.214%
27	17.381	2440	2447	2459	rVV2	1216288	1754595	79.11%	9.634%
28	17.486	2462	2465	2473	rVB5	5249	7305	0.33%	0.040%
29	18.169	2577	2581	2588	rBV	12551	16588	0.75%	0.091%
30	19.245	2760	2764	2769	rBV2	12847	16885	0.76%	0.093%
31	19.316	2772	2776	2780	rBV	12645	15316	0.69%	0.084%
32	19.457	2797	2800	2808	rBV6	12330	17423	0.79%	0.096%
33	19.610	2822	2826	2832	rBV5	4021	5917	0.27%	0.032%
34	19.680	2832	2838	2847	rBV	1458227	1994452	89.92%	10.951%
35	20.222	2928	2930	2932	rBV2	3597	2511	0.11%	0.014%
36	21.486	3139	3145	3153	rBV	832177	1103602	49.76%	6.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022754.D
Acq On : 18 Nov 2022 13:23
Operator : CG/JU
Sample : N5689-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.727	3518	3526	3539	rVB2	1093806	2217985	100.00%	12.179%
38	23.886	3545	3553	3562	rVB2	553758	1126759	50.80%	6.187%




Sum of corrected areas: 18212273

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022754.D
Acq On : 18 Nov 2022 13:23
Operator : CG/JU
Sample : N5689-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

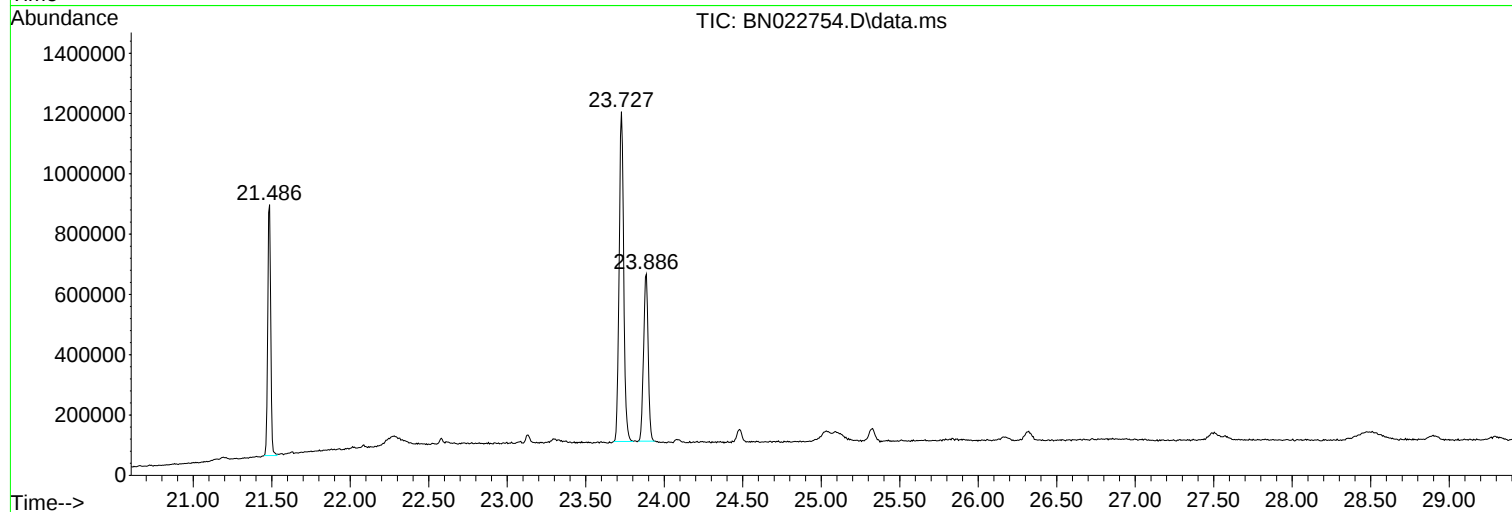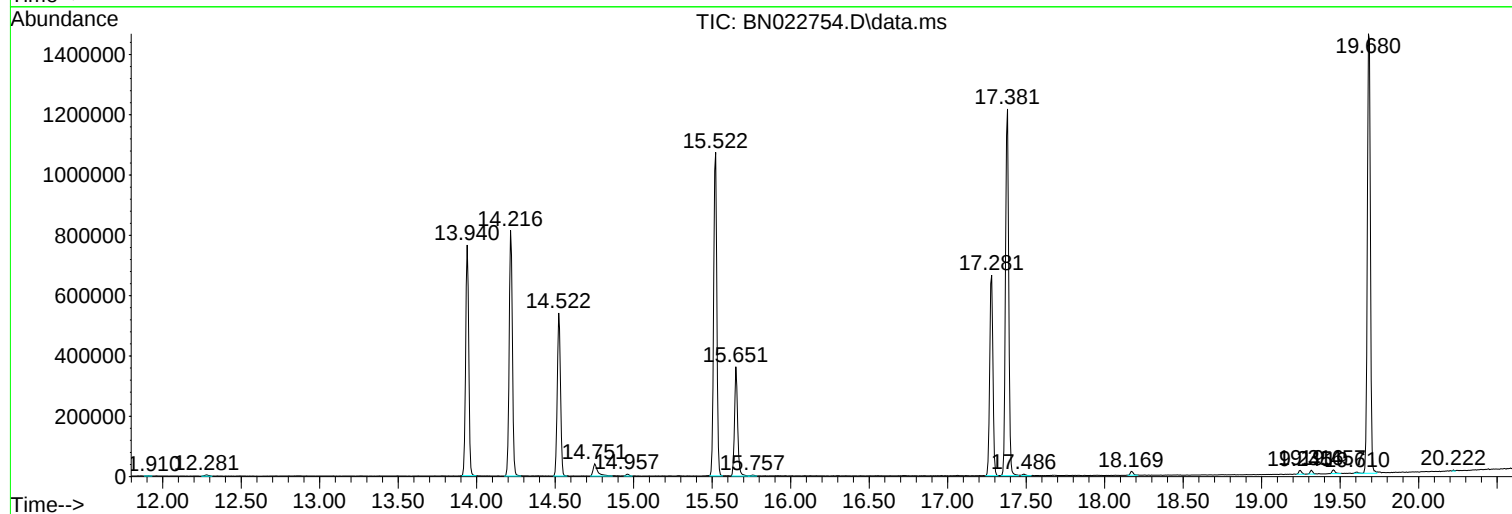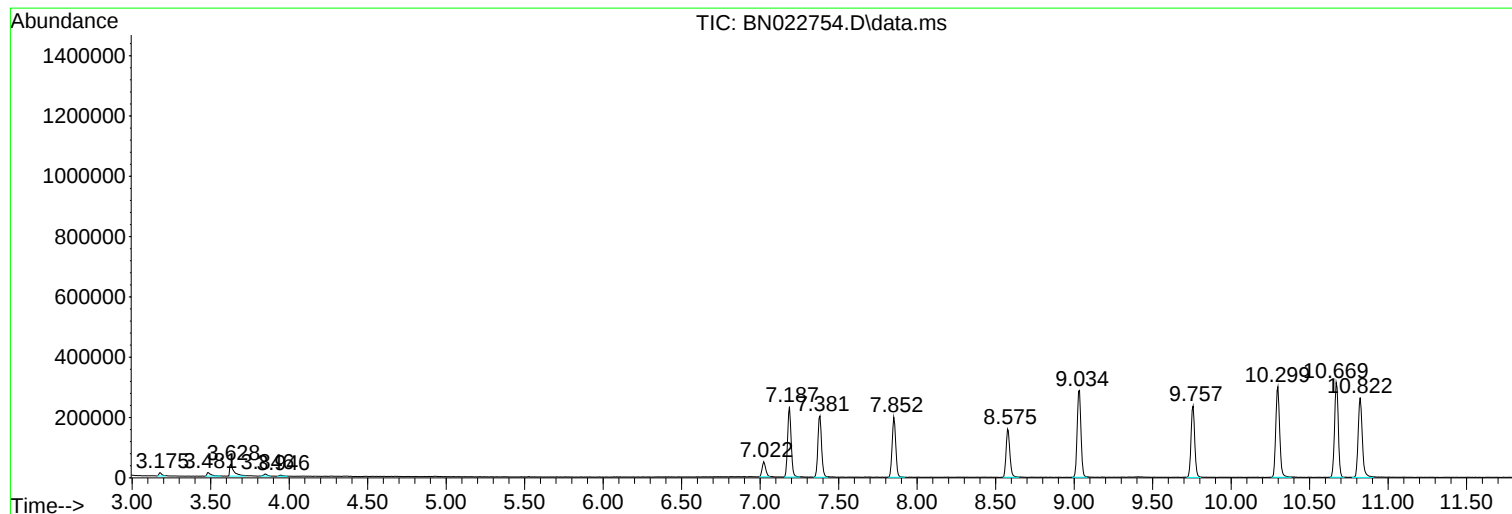

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022754.D
Acq On : 18 Nov 2022 13:23
Operator : CG/JU
Sample : N5689-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022754.D
Acq On : 18 Nov 2022 13:23
Operator : CG/JU
Sample : N5689-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
