

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022758.D
 Acq On : 18 Nov 2022 15:50
 Operator : CG/JU
 Sample : N5689-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	40	rVB	10337	15785	0.65%	0.083%
2	3.487	82	85	92	rBV	6543	10188	0.42%	0.054%
3	3.623	106	108	123	rBV	37458	72506	3.00%	0.383%
4	3.846	142	146	154	rVB2	6851	11964	0.49%	0.063%
5	3.952	159	164	170	rVB2	2920	5206	0.22%	0.027%
6	7.022	679	686	698	rVB	58442	98021	4.05%	0.518%
7	7.187	707	714	726	rBV	239584	383736	15.86%	2.026%
8	7.381	740	747	758	rBV	216376	354895	14.67%	1.874%
9	7.852	821	827	837	rBV	187798	293801	12.14%	1.551%
10	8.575	944	950	967	rVB	184101	304449	12.58%	1.607%
11	9.034	1019	1028	1042	rBV	309453	521080	21.54%	2.751%
12	9.152	1044	1048	1052	rVB4	1864	2931	0.12%	0.015%
13	9.410	1086	1092	1098	rBV5	1250	2520	0.10%	0.013%
14	9.758	1144	1151	1160	rBV	261048	421756	17.43%	2.227%
15	10.293	1236	1242	1253	rBV	330940	570792	23.59%	3.014%
16	10.669	1299	1306	1315	rBV	304156	490921	20.29%	2.592%
17	10.822	1325	1332	1349	rBV	333234	586460	24.24%	3.096%
18	12.275	1575	1579	1589	rVB3	3587	7123	0.29%	0.038%
19	13.940	1850	1862	1873	rBV	798683	1110053	45.89%	5.861%
20	14.216	1903	1909	1922	rBV	882592	1246214	51.51%	6.580%
21	14.522	1955	1961	1972	rBV	506907	725128	29.97%	3.829%
22	14.751	1993	2000	2015	rBV	49279	98023	4.05%	0.518%
23	14.963	2033	2036	2039	rVB3	2804	2717	0.11%	0.014%
24	15.516	2124	2130	2140	rBV	1116872	1609380	66.53%	8.497%
25	15.651	2148	2153	2167	rVV	400302	546680	22.60%	2.886%
26	15.763	2167	2172	2177	rVB2	3343	4556	0.19%	0.024%
27	17.281	2423	2430	2438	rBV	634487	903833	37.36%	4.772%
28	17.381	2440	2447	2461	rVV	1226600	1781251	73.63%	9.405%
29	18.169	2577	2581	2591	rBV2	15717	22134	0.91%	0.117%
30	19.245	2760	2764	2770	rBV3	13812	18594	0.77%	0.098%
31	19.316	2772	2776	2778	rBV2	13846	18257	0.75%	0.096%
32	19.457	2797	2800	2804	rBV2	16893	22586	0.93%	0.119%
33	19.604	2822	2825	2830	rBV5	3639	6057	0.25%	0.032%
34	19.686	2832	2839	2846	rBV	1503576	2058963	85.11%	10.871%
35	21.486	3140	3145	3152	rBV	837517	1065536	44.05%	5.626%
36	23.727	3519	3526	3542	rVB2	1165168	2419173	100.00%	12.773%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022758.D
Acq On : 18 Nov 2022 15:50
Operator : CG/JU
Sample : N5689-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.886	3546	3553	3562	rVB2	574956	1126951	46.58%	5.950%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 18940220

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022758.D
Acq On : 18 Nov 2022 15:50
Operator : CG/JU
Sample : N5689-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

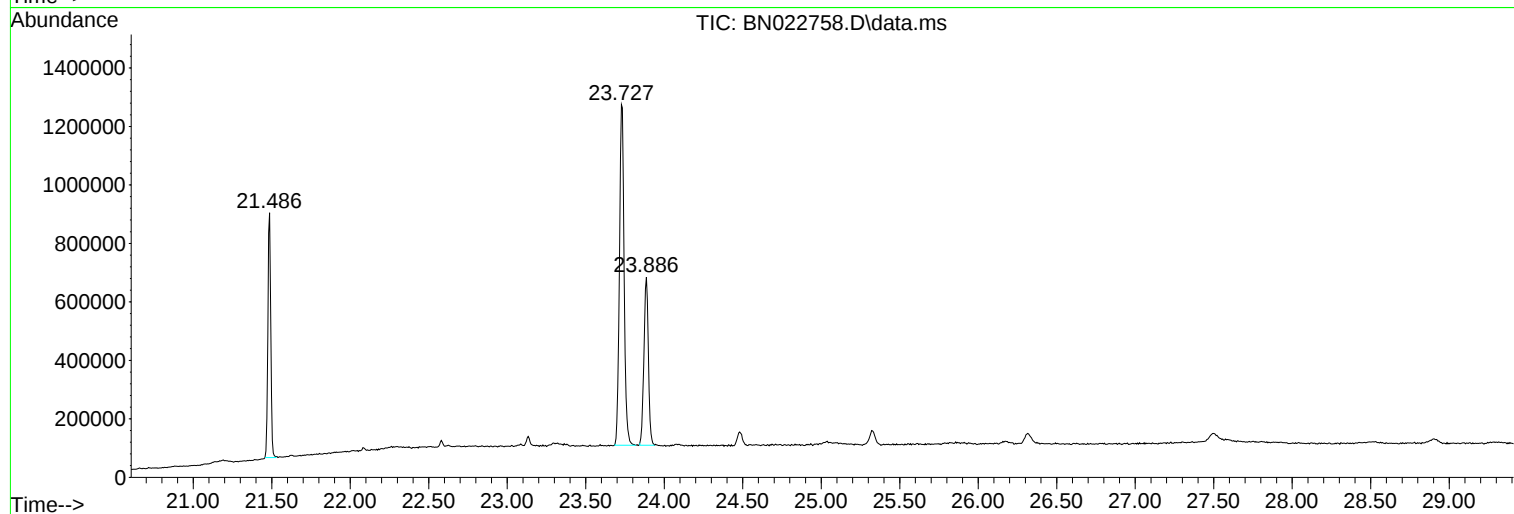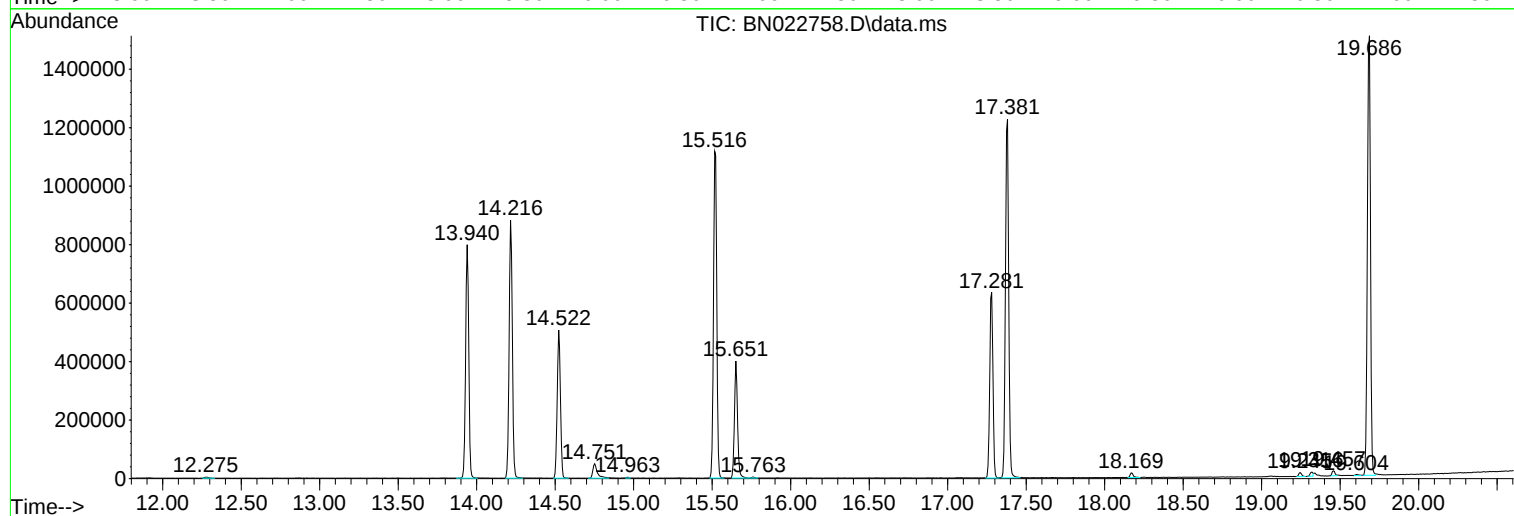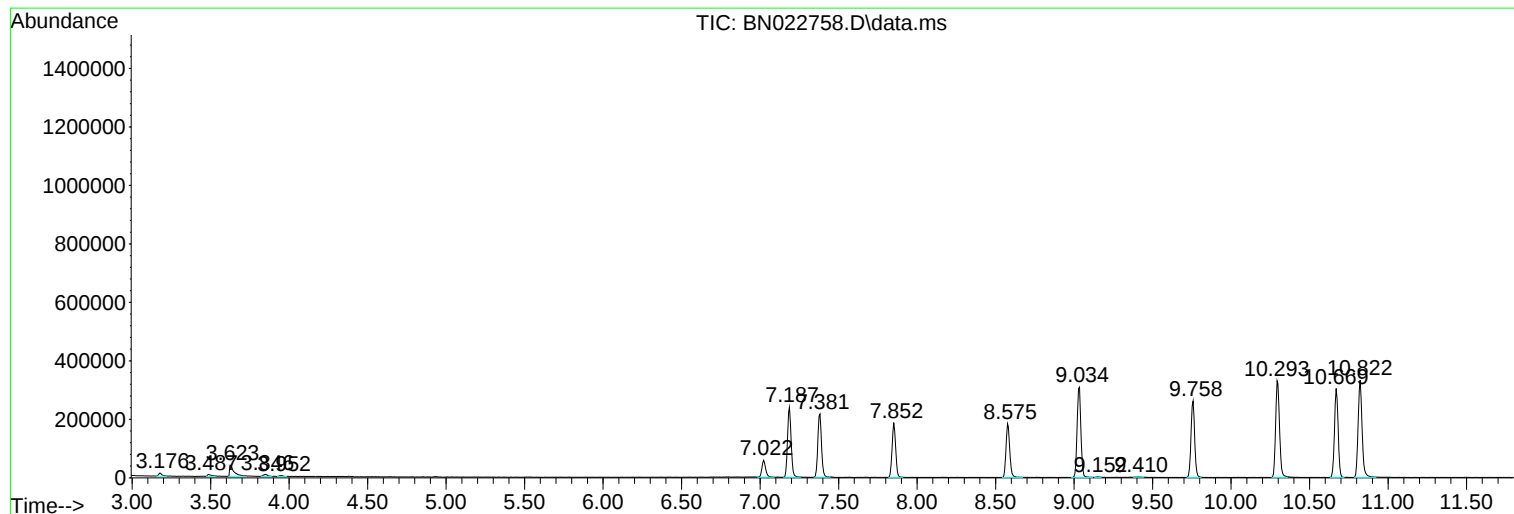

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022758.D
Acq On : 18 Nov 2022 15:50
Operator : CG/JU
Sample : N5689-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022758.D
Acq On : 18 Nov 2022 15:50
Operator : CG/JU
Sample : N5689-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
