

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022764.D
 Acq On : 18 Nov 2022 20:10
 Operator : CG/JU
 Sample : PB149167BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	43	rVB	16949	26017	1.20%	0.125%
2	3.617	104	107	124	rBV	200707	342875	15.77%	1.645%
3	3.952	159	164	168	rBV2	4082	6474	0.30%	0.031%
4	7.022	680	686	697	rBV	267327	435635	20.04%	2.091%
5	7.187	706	714	724	rBV	224316	348895	16.05%	1.674%
6	7.375	740	746	760	rVB	258783	429631	19.76%	2.062%
7	7.852	821	827	839	rBV	236124	374973	17.25%	1.799%
8	8.575	944	950	965	rBV	336246	558224	25.68%	2.679%
9	9.034	1021	1028	1037	rBV	272584	455951	20.97%	2.188%
10	9.757	1144	1151	1161	rBV	237498	389081	17.90%	1.867%
11	10.299	1234	1243	1260	rBV	324835	568333	26.14%	2.727%
12	10.669	1299	1306	1314	rVB	364430	608103	27.97%	2.918%
13	10.822	1323	1332	1351	rBV	349815	627770	28.87%	3.013%
14	12.281	1575	1580	1586	rBV2	3275	5986	0.28%	0.029%
15	13.940	1849	1862	1873	rBV	748288	996782	45.85%	4.783%
16	14.216	1902	1909	1922	rBV	753202	1088032	50.05%	5.221%
17	14.522	1953	1961	1970	rBV	616661	893747	41.11%	4.289%
18	14.745	1992	1999	2026	rBV	317031	551386	25.36%	2.646%
19	15.292	2083	2092	2095	rBV5	1009	2703	0.12%	0.013%
20	15.522	2124	2131	2138	rVV	977623	1397727	64.29%	6.708%
21	15.651	2147	2153	2167	rBV	353696	499167	22.96%	2.395%
22	15.757	2167	2171	2176	rVB3	2581	3794	0.17%	0.018%
23	17.281	2424	2430	2438	rVB	773704	1098796	50.54%	5.273%
24	17.375	2440	2446	2464	rVB2	1086743	1594582	73.34%	7.652%
25	18.739	2676	2678	2684	rBV5	1434	2375	0.11%	0.011%
26	19.010	2721	2724	2727	rBV4	1883	3000	0.14%	0.014%
27	19.245	2760	2764	2768	rVB2	11209	13551	0.62%	0.065%
28	19.316	2772	2776	2780	rVV2	10357	12438	0.57%	0.060%
29	19.604	2823	2825	2828	rVB3	2489	2292	0.11%	0.011%
30	19.680	2832	2838	2848	rBV2	1347560	1838029	84.54%	8.820%
31	20.651	3001	3003	3004	rBV2	4759	2792	0.13%	0.013%
32	21.480	3139	3144	3154	rVB	1041948	1288078	59.25%	6.181%
33	23.292	3448	3452	3461	rVB2	59552	116356	5.35%	0.558%
34	23.721	3518	3525	3537	rVB2	1047806	2174099	100.00%	10.433%
35	23.880	3544	3552	3561	rVB2	657899	1360831	62.59%	6.530%
36	24.080	3582	3586	3595	rVB4	76892	159797	7.35%	0.767%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	24.474	3649	3653	3659	rVB2	60999	111286	5.12%	0.534%
38	25.021	3740	3746	3769	rVB3	113072	448625	20.63%	2.153%


Sum of corrected areas: 20838213

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

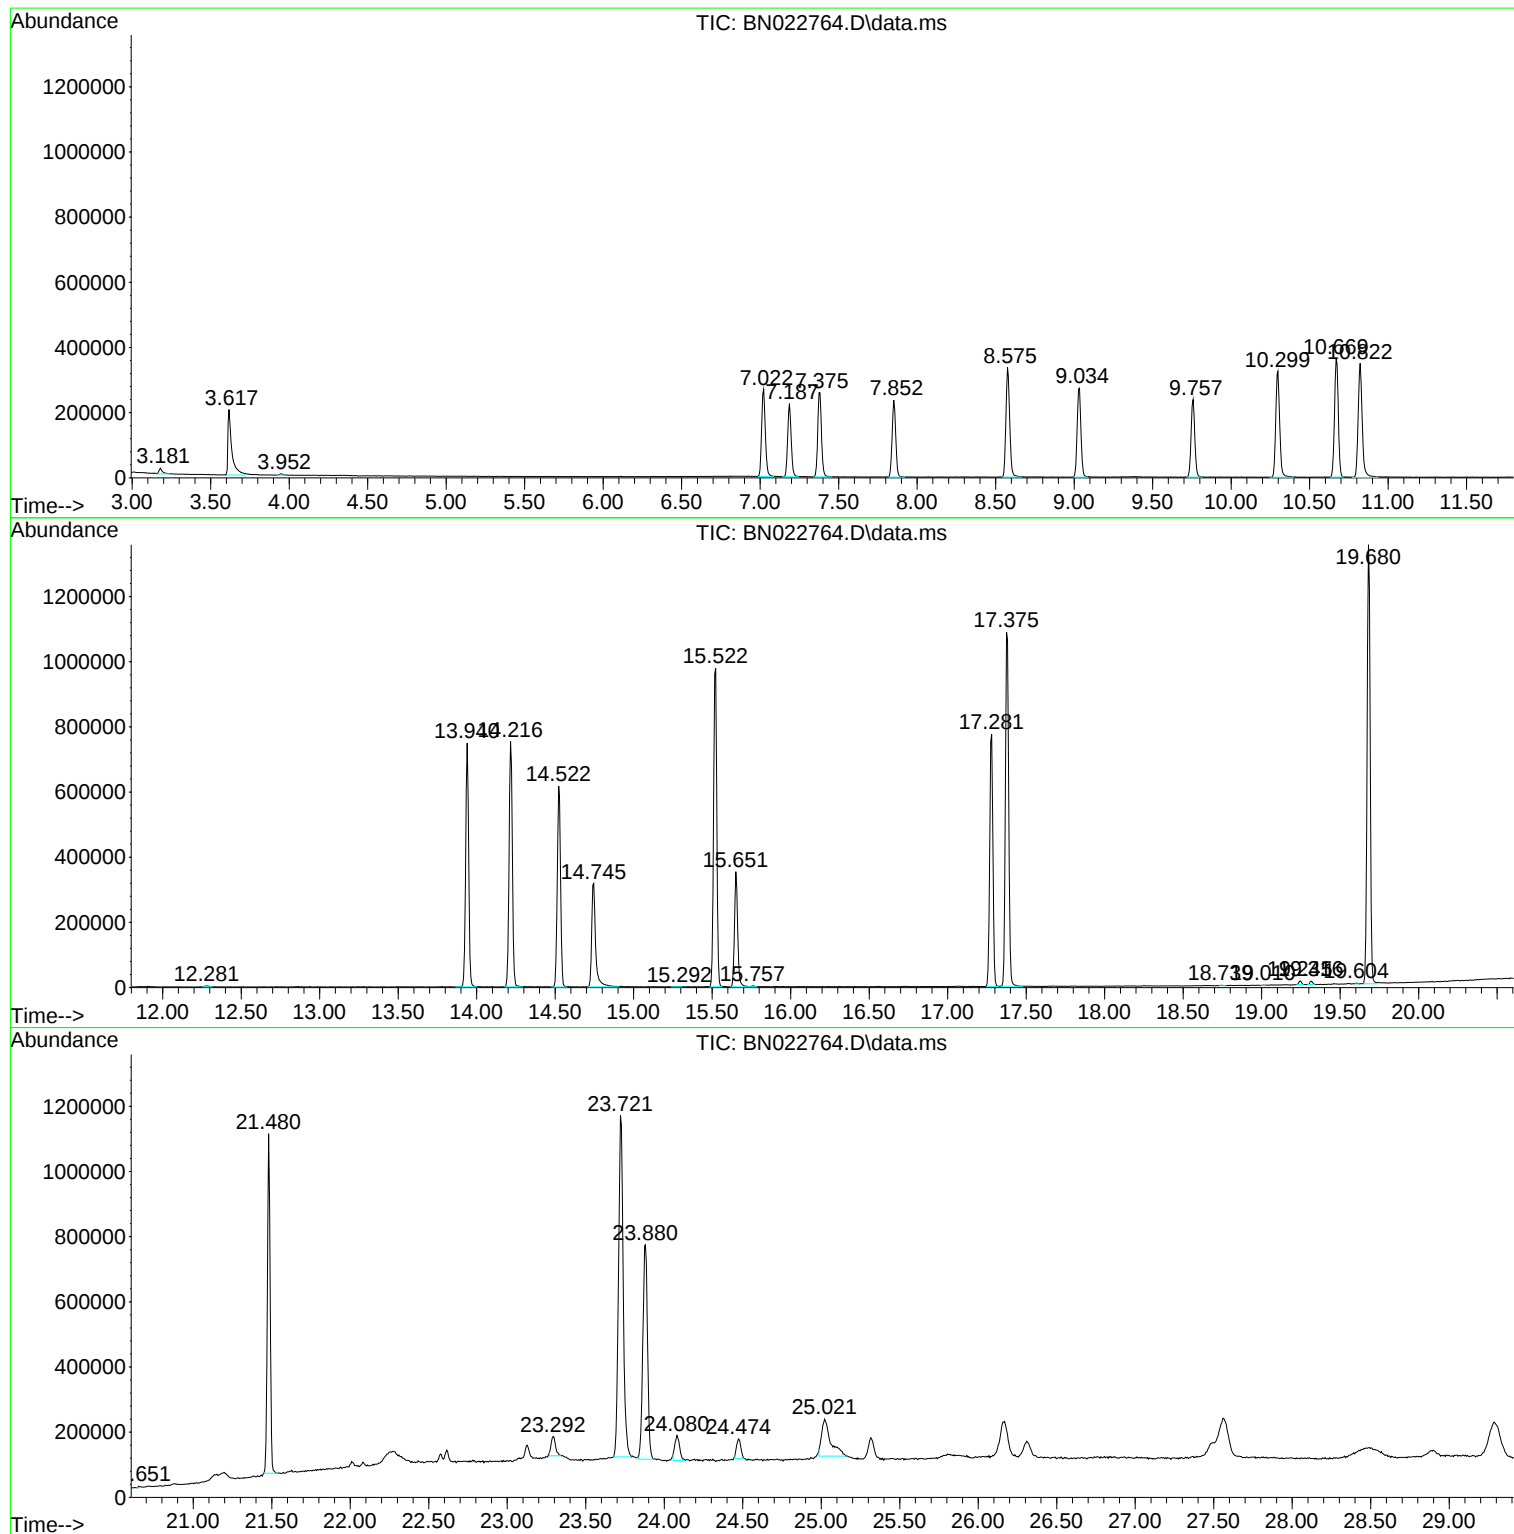

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.080	2.35 ng/ul	159797	Perylene-d12	23.880

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3,6-Dioxa-2,4,5,7-tetrasilaoctan...	294	C10H30O2Si4	004342-25-0	40
2			Trimethylsilyl 4-propylbenzoate	236	C13H20O2Si	1000408-13-2	38
3			1,1,1,5,7,7,7-Heptamethyl-3,3-bi...	444	C13H40O5Si6	038147-00-1	37
4			N-Benzyl-N-ethyl-p-isopropylbenz...	281	C19H23NO	015089-22-2	25
5			Mercaptoacetic acid, 2TMS deriva...	236	C8H20O2SSi2	006398-62-5	25

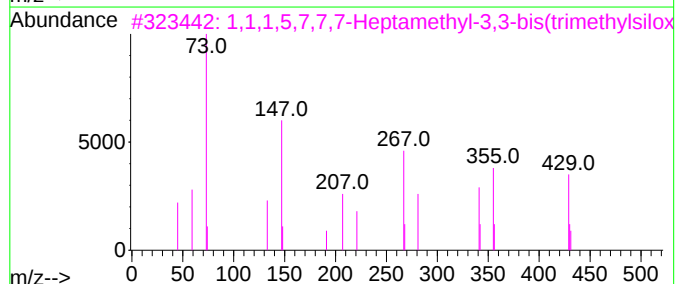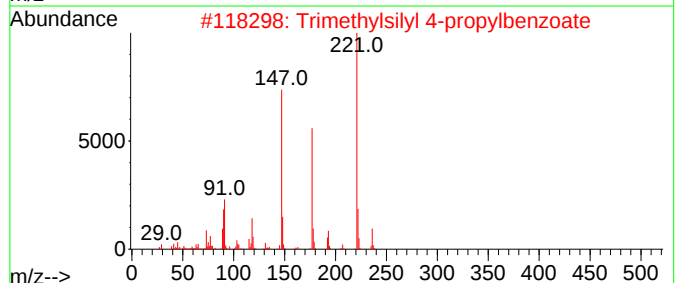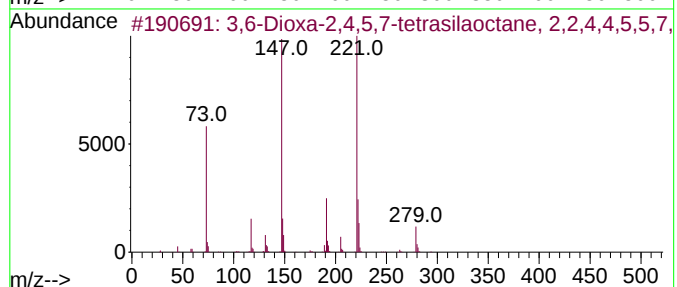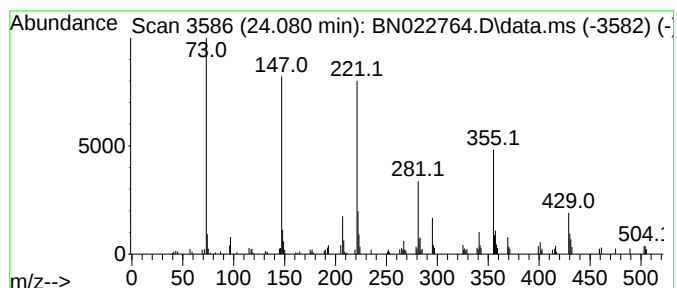

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Hexasiloxane, tetradecamethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.021	6.59 ng/ul	448625	Perylene-d12	23.880

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	81
2			Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	50
3			2-Amino-2-oxo-acetic acid, N-[3,...	221	C12H15NO3	024451-17-0	37
4			3,6-Dioxa-2,4,5,7-tetrasilaoctan...	294	C10H30O2Si4	004342-25-0	37
5			Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	33

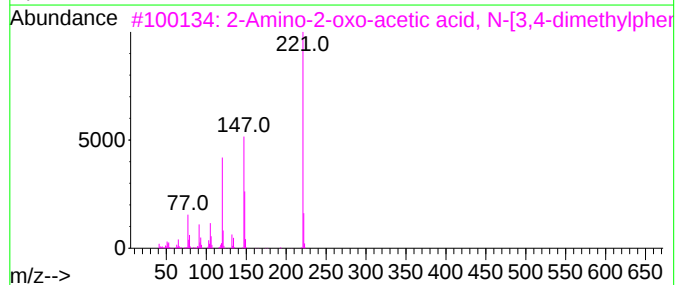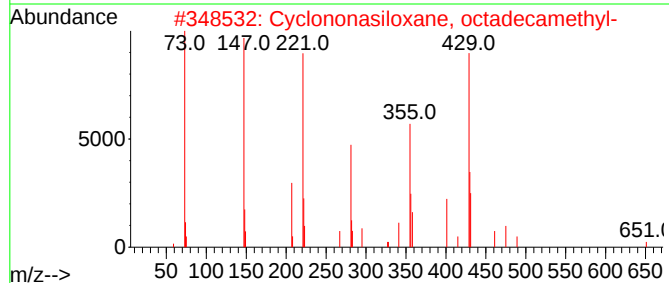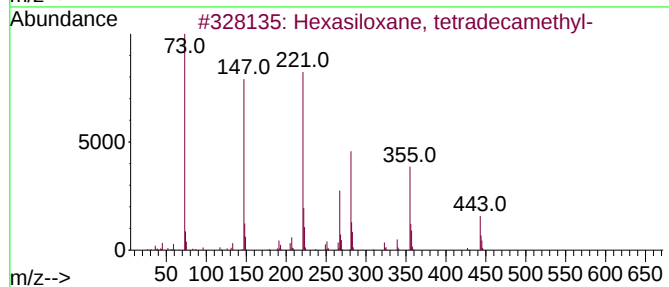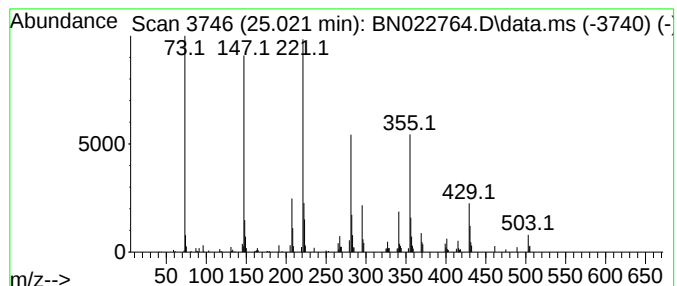

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022764.D
Acq On : 18 Nov 2022 20:10
Operator : CG/JU
Sample : PB149167BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK167

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	24.080	2.4	ng/u1	159797	6	23.880	1360830	20.0
Hexasiloxane, t...	25.021	6.6	ng/u1	448625	6	23.880	1360830	20.0