

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022765.D
 Acq On : 18 Nov 2022 20:47
 Operator : CG/JU
 Sample : PB149169BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	41	rBV	16290	23564	1.13%	0.124%
2	3.617	103	107	132	rBV	196746	364393	17.50%	1.911%
3	3.952	159	164	170	rBV3	3331	6240	0.30%	0.033%
4	4.311	221	225	228	rBV5	1328	2300	0.11%	0.012%
5	7.022	679	686	706	rVB	277512	446428	21.43%	2.341%
6	7.187	706	714	732	rVB	226916	359671	17.27%	1.886%
7	7.375	740	746	761	rBV	262484	431620	20.72%	2.263%
8	7.852	820	827	838	rVB	206331	326616	15.68%	1.713%
9	8.575	944	950	968	rBV	356446	573606	27.54%	3.008%
10	9.034	1017	1028	1042	rBV	278011	473129	22.72%	2.481%
11	9.758	1144	1151	1160	rBV	240305	395128	18.97%	2.072%
12	10.293	1235	1242	1262	rBV	334517	571257	27.43%	2.995%
13	10.669	1299	1306	1316	rBV	322547	531488	25.52%	2.787%
14	10.822	1325	1332	1352	rBV	355864	634278	30.45%	3.326%
15	12.281	1571	1580	1587	rVB4	3388	7202	0.35%	0.038%
16	13.940	1855	1862	1876	rVB	726325	1004954	48.25%	5.269%
17	14.216	1902	1909	1919	rBV2	772646	1090793	52.37%	5.719%
18	14.522	1955	1961	1970	rVB	542752	779178	37.41%	4.085%
19	14.746	1993	1999	2019	rBV	319584	536933	25.78%	2.815%
20	15.516	2124	2130	2138	rVV	1005647	1401766	67.30%	7.350%
21	15.651	2147	2153	2165	rBV	362908	493870	23.71%	2.589%
22	15.757	2168	2171	2176	rVB3	3339	4144	0.20%	0.022%
23	17.069	2390	2394	2397	rBV3	1243	2312	0.11%	0.012%
24	17.275	2423	2429	2437	rBV	661974	941997	45.23%	4.939%
25	17.375	2440	2446	2460	rBV	1070598	1575425	75.64%	8.260%
26	19.245	2760	2764	2770	rVB2	11072	15220	0.73%	0.080%
27	19.316	2772	2776	2780	rBV2	9783	12695	0.61%	0.067%
28	19.681	2832	2838	2847	rBV	1371944	1809733	86.89%	9.489%
29	21.480	3139	3144	3151	rBV	862717	1061637	50.97%	5.566%
30	23.722	3517	3525	3540	rVB2	994251	2082810	100.00%	10.921%
31	23.874	3544	3551	3560	rVB	541188	1111672	53.37%	5.829%




Sum of corrected areas: 19072059

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022765.D
Acq On : 18 Nov 2022 20:47
Operator : CG/JU
Sample : PB149169BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

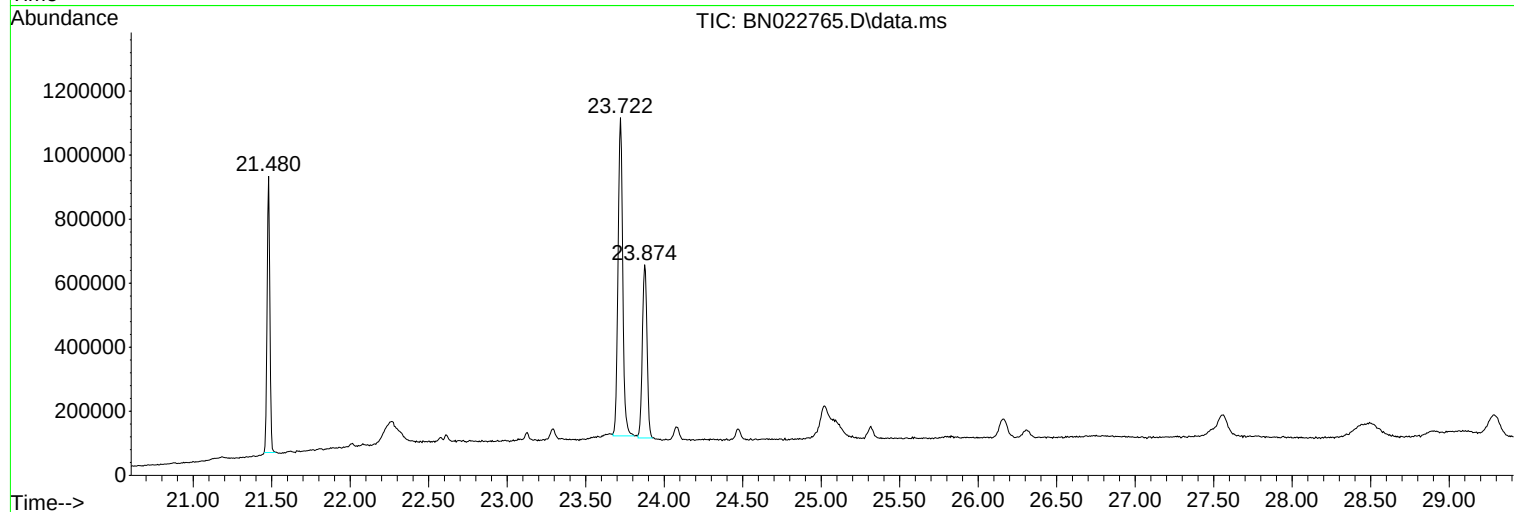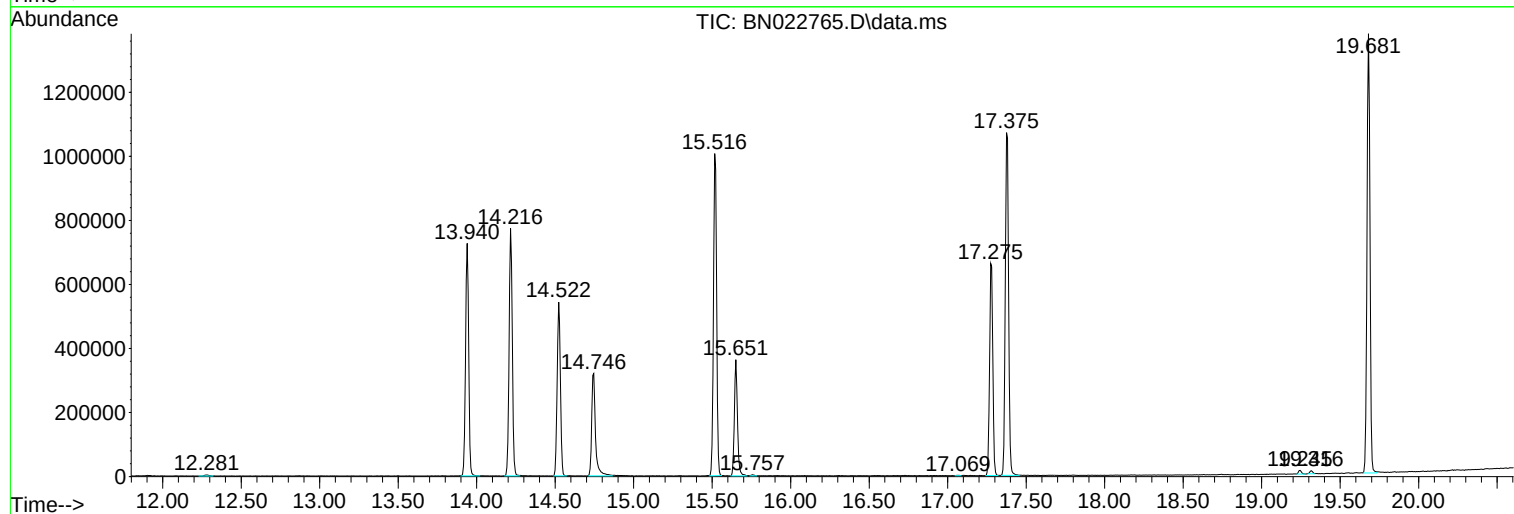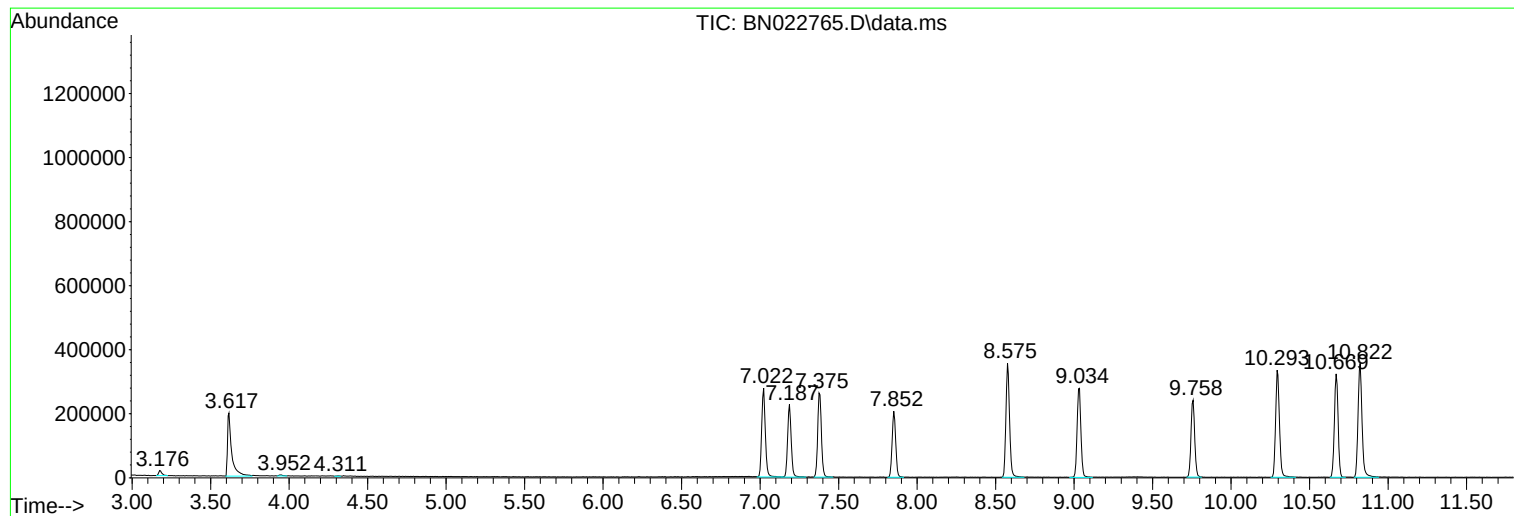

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022765.D
Acq On : 18 Nov 2022 20:47
Operator : CG/JU
Sample : PB149169BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022765.D
Acq On : 18 Nov 2022 20:47
Operator : CG/JU
Sample : PB149169BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK169

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc