

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022766.D
 Acq On : 18 Nov 2022 21:24
 Operator : CG/JU
 Sample : N5689-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	40	rVB2	6241	8824	0.38%	0.049%
2	3.640	108	111	125	rBV	14682	31903	1.39%	0.177%
3	3.846	141	146	151	rBV	7182	10473	0.46%	0.058%
4	3.946	160	163	167	rBV2	3241	4285	0.19%	0.024%
5	4.934	327	331	336	rVB2	1952	2825	0.12%	0.016%
6	7.022	678	686	696	rBV	58298	96688	4.20%	0.535%
7	7.187	704	714	723	rBV	247002	387603	16.85%	2.146%
8	7.381	740	747	758	rBV	222535	366002	15.91%	2.026%
9	7.852	820	827	835	rBV	186862	291210	12.66%	1.612%
10	8.575	944	950	960	rBV	183084	300977	13.08%	1.666%
11	9.034	1020	1028	1037	rBV	309284	514621	22.37%	2.849%
12	9.404	1088	1091	1096	rVB3	1802	2802	0.12%	0.016%
13	9.757	1144	1151	1163	rVB	257660	421112	18.30%	2.331%
14	10.298	1236	1243	1254	rBV	320306	568947	24.73%	3.149%
15	10.669	1299	1306	1314	rBV	292186	480480	20.88%	2.660%
16	10.822	1325	1332	1347	rBV	106528	205909	8.95%	1.140%
17	11.904	1513	1516	1523	rVB4	1374	2803	0.12%	0.016%
18	12.275	1574	1579	1586	rVB4	4092	8170	0.36%	0.045%
19	13.786	1830	1836	1841	rBV5	1153	2321	0.10%	0.013%
20	13.939	1853	1862	1876	rBV	803882	1091816	47.45%	6.044%
21	14.216	1902	1909	1923	rBV	859304	1230423	53.48%	6.811%
22	14.522	1953	1961	1972	rBV	492690	706253	30.70%	3.910%
23	14.751	1994	2000	2015	rBV	47815	96165	4.18%	0.532%
24	14.963	2033	2036	2040	rVB5	2722	2590	0.11%	0.014%
25	15.516	2124	2130	2139	rVV	1081041	1572535	68.35%	8.705%
26	15.651	2147	2153	2166	rVB	398919	534297	23.22%	2.958%
27	15.757	2168	2171	2176	rVB2	3484	4276	0.19%	0.024%
28	17.275	2423	2429	2436	rBV	612355	859413	37.35%	4.757%
29	17.375	2440	2446	2463	rVB2	1229018	1770891	76.97%	9.803%
30	18.169	2577	2581	2587	rBV3	13786	17060	0.74%	0.094%
31	19.245	2760	2764	2768	rBV	13164	15966	0.69%	0.088%
32	19.316	2772	2776	2782	rVB3	10936	15393	0.67%	0.085%
33	19.457	2796	2800	2806	rBV5	11373	17683	0.77%	0.098%
34	19.680	2832	2838	2849	rBV	1565382	2030451	88.25%	11.240%
35	21.480	3139	3144	3155	rBV	789874	1017102	44.21%	5.630%
36	23.721	3518	3525	3541	rVB2	1126311	2300765	100.00%	12.736%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022766.D
Acq On : 18 Nov 2022 21:24
Operator : CG/JU
Sample : N5689-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.874	3545	3551	3562	rVB2	521447	1073783	46.67%	5.944%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 18064817

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022766.D
Acq On : 18 Nov 2022 21:24
Operator : CG/JU
Sample : N5689-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

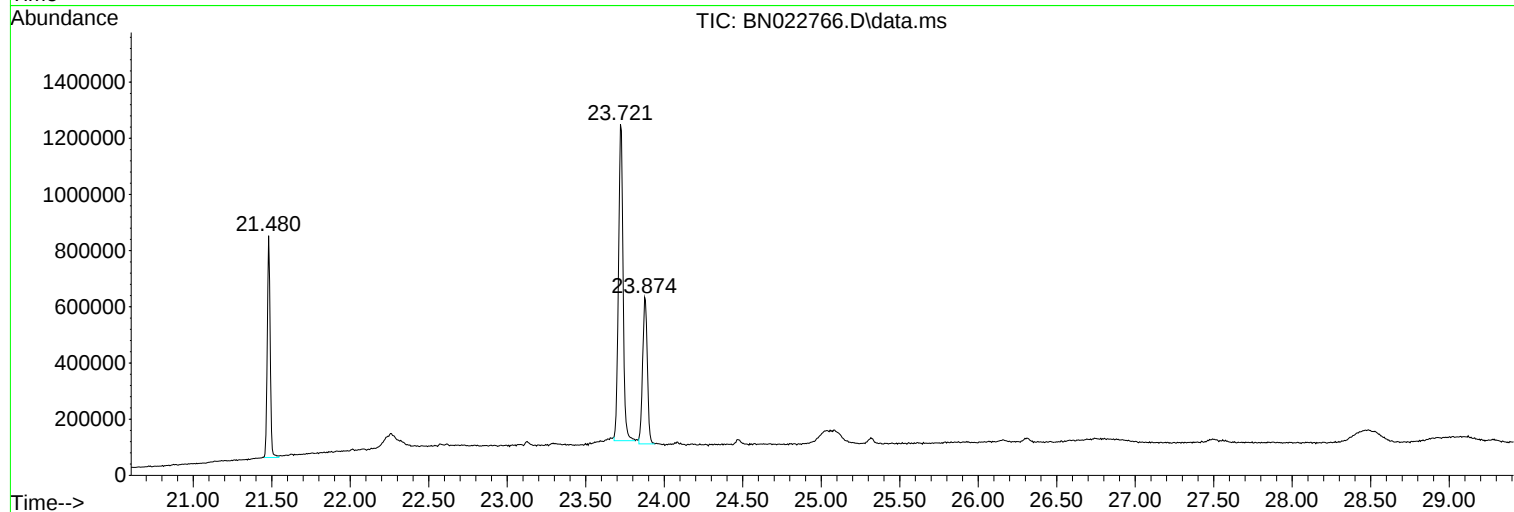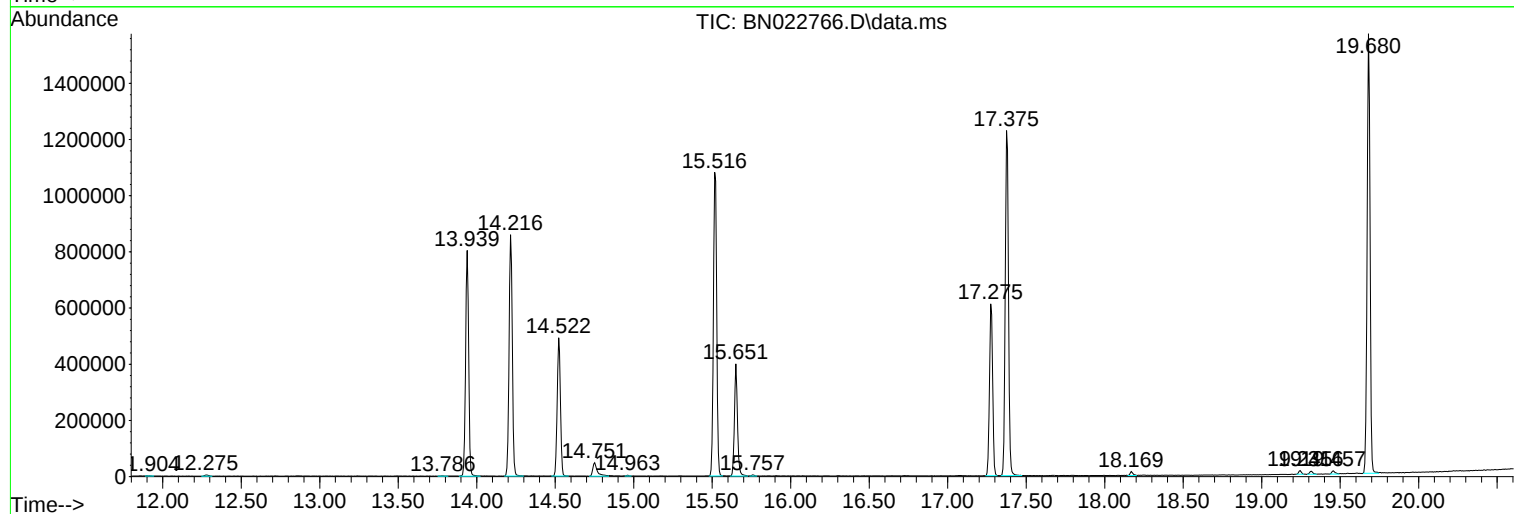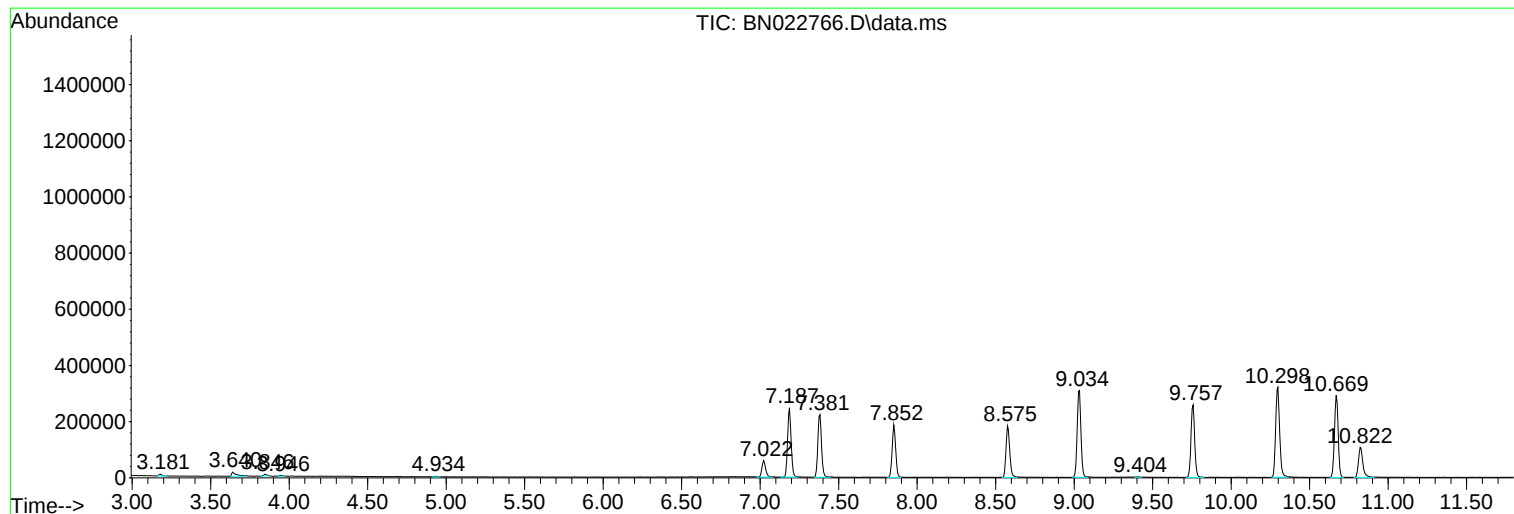

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022766.D
Acq On : 18 Nov 2022 21:24
Operator : CG/JU
Sample : N5689-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022766.D
Acq On : 18 Nov 2022 21:24
Operator : CG/JU
Sample : N5689-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc