

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022768.D
 Acq On : 18 Nov 2022 22:37
 Operator : CG/JU
 Sample : N5689-13
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	41	rVB	7219	12349	0.51%	0.062%
2	3.628	107	109	129	rBV	36232	75624	3.12%	0.382%
3	3.846	142	146	155	rVB	7259	13360	0.55%	0.067%
4	3.946	159	163	166	rBV3	3189	4376	0.18%	0.022%
5	4.940	328	332	337	rVB5	1590	2975	0.12%	0.015%
6	7.022	680	686	696	rVB	69519	112004	4.63%	0.565%
7	7.187	707	714	723	rBV	259174	414203	17.11%	2.091%
8	7.375	739	746	757	rBV	247558	406791	16.80%	2.054%
9	7.852	820	827	839	rBV	208574	340012	14.04%	1.717%
10	8.575	944	950	963	rBV	218191	351550	14.52%	1.775%
11	9.028	1021	1027	1038	rBV	333816	554186	22.89%	2.798%
12	9.410	1087	1092	1098	rVB5	1948	4563	0.19%	0.023%
13	9.757	1142	1151	1163	rBV	272393	459256	18.97%	2.319%
14	10.293	1234	1242	1257	rBV	364146	632331	26.12%	3.192%
15	10.669	1299	1306	1318	rVB	333829	551232	22.77%	2.783%
16	10.822	1324	1332	1349	rBV	100025	196743	8.13%	0.993%
17	12.275	1575	1579	1588	rVB3	4909	8914	0.37%	0.045%
18	13.940	1852	1862	1870	rBV	841134	1173428	48.47%	5.924%
19	14.216	1902	1909	1922	rBV	945174	1320019	54.52%	6.664%
20	14.522	1952	1961	1968	rBV	575681	810711	33.49%	4.093%
21	14.745	1994	1999	2018	rBV	57256	121485	5.02%	0.613%
22	15.516	2124	2130	2140	rBV	1188208	1688529	69.75%	8.525%
23	15.651	2147	2153	2166	rBV	433882	594412	24.55%	3.001%
24	15.763	2168	2172	2177	rVB2	3781	4502	0.19%	0.023%
25	17.275	2423	2429	2436	rBV	701070	972353	40.16%	4.909%
26	17.375	2440	2446	2462	rBV	1334517	1926586	79.58%	9.726%
27	18.169	2575	2581	2588	rBV	36004	50081	2.07%	0.253%
28	19.239	2760	2763	2768	rVV	15129	20549	0.85%	0.104%
29	19.316	2771	2776	2781	rBV	14233	20288	0.84%	0.102%
30	19.457	2796	2800	2808	rBV	36854	54470	2.25%	0.275%
31	19.598	2822	2824	2827	rBV4	2836	3118	0.13%	0.016%
32	19.680	2832	2838	2852	rVV	1618035	2169558	89.61%	10.953%
33	21.480	3139	3144	3153	rVB2	867928	1098310	45.37%	5.545%
34	23.292	3448	3452	3461	rVB3	40501	83824	3.46%	0.423%
35	23.721	3518	3525	3539	rVB2	1225890	2420995	100.00%	12.222%
36	23.880	3545	3552	3562	rVB2	565058	1134138	46.85%	5.726%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022768.D
Acq On : 18 Nov 2022 22:37
Operator : CG/JU
Sample : N5689-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 19807825

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022768.D
Acq On : 18 Nov 2022 22:37
Operator : CG/JU
Sample : N5689-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

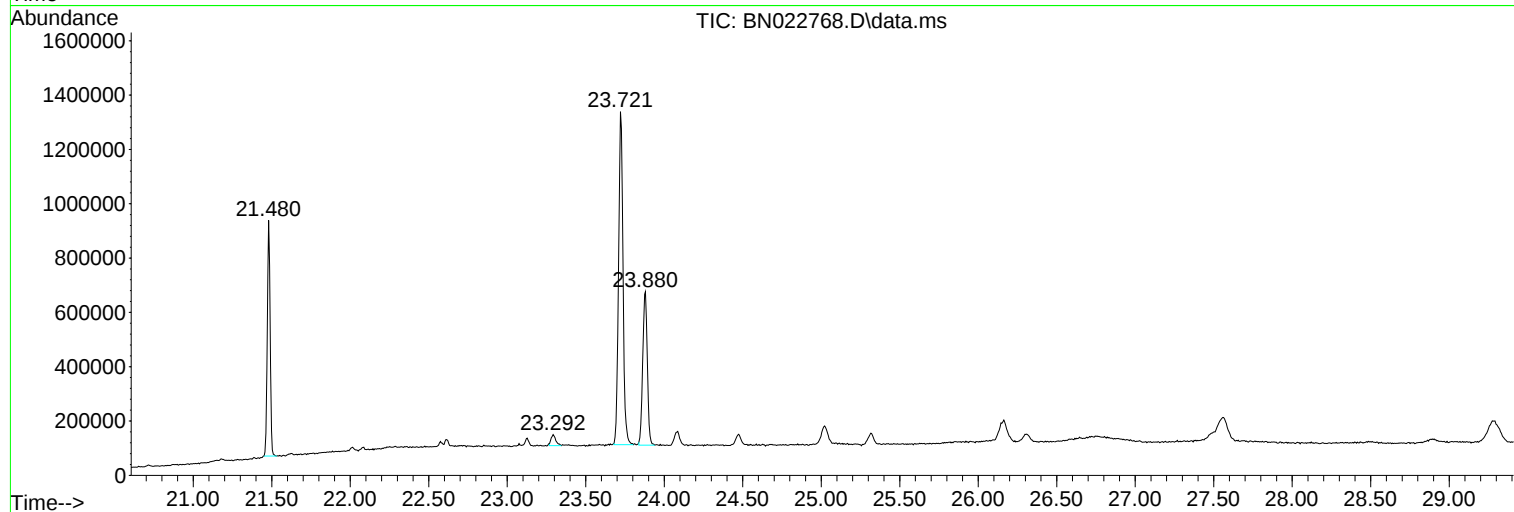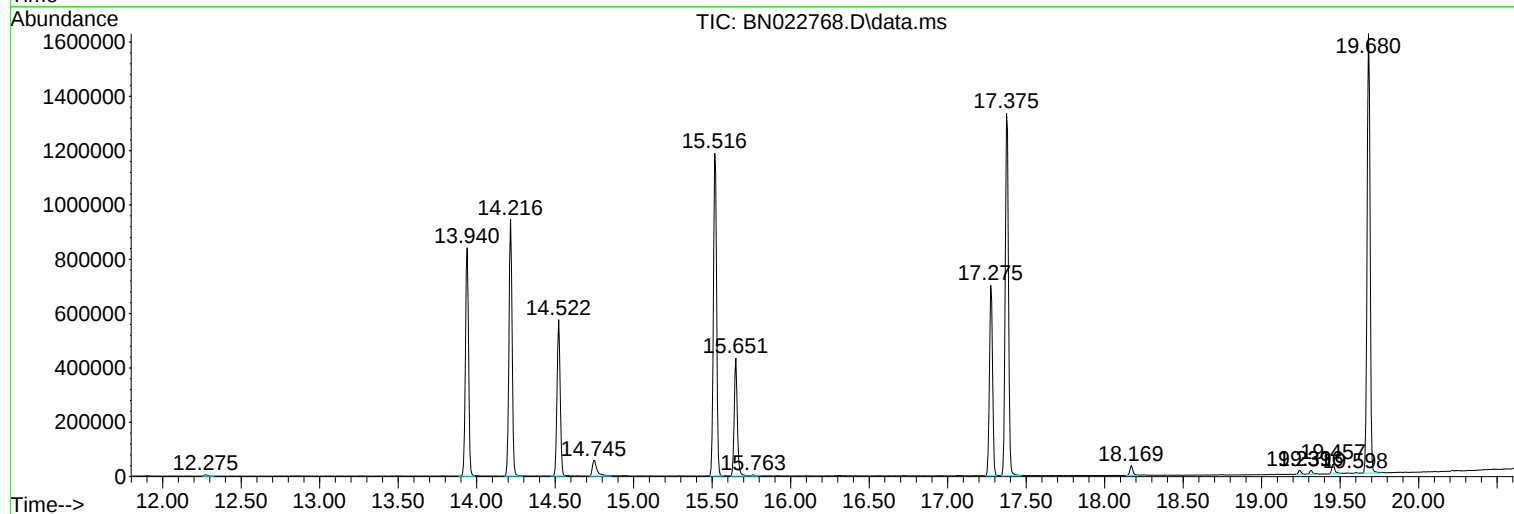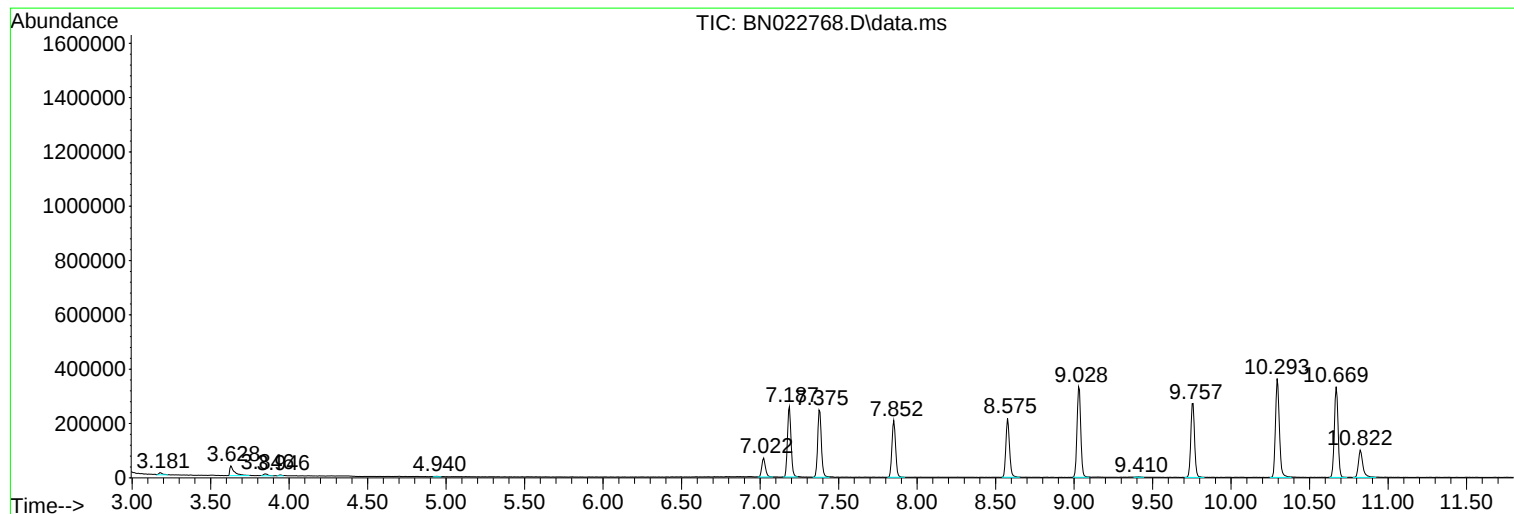

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022768.D
Acq On : 18 Nov 2022 22:37
Operator : CG/JU
Sample : N5689-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022768.D
Acq On : 18 Nov 2022 22:37
Operator : CG/JU
Sample : N5689-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
