

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022773.D
 Acq On : 19 Nov 2022 01:40
 Operator : CG/JU
 Sample : N5689-18
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	38	rVB2	7142	10101	0.41%	0.049%
2	3.487	82	85	95	rVB	9415	16826	0.68%	0.082%
3	3.628	107	109	122	rBV	43059	80380	3.26%	0.393%
4	3.846	142	146	153	rVB	8416	14731	0.60%	0.072%
5	3.946	160	163	166	rVB2	3517	3901	0.16%	0.019%
6	4.922	325	329	339	rVB	5023	9647	0.39%	0.047%
7	7.022	680	686	694	rBV	51417	83735	3.39%	0.410%
8	7.181	707	713	723	rBV	258390	422418	17.11%	2.067%
9	7.375	740	746	757	rBV	174446	285239	11.55%	1.396%
10	7.852	820	827	838	rBV	239800	385330	15.61%	1.886%
11	8.575	944	950	964	rBV	156234	253423	10.26%	1.240%
12	9.028	1021	1027	1037	rBV	340849	561464	22.74%	2.748%
13	9.751	1144	1150	1163	rBV	185247	310659	12.58%	1.520%
14	10.293	1236	1242	1257	rBV	252570	433332	17.55%	2.121%
15	10.669	1298	1306	1315	rBV	373222	621428	25.17%	3.041%
16	10.816	1324	1331	1348	rBV	346075	626146	25.36%	3.064%
17	12.275	1575	1579	1588	rVB3	5093	9794	0.40%	0.048%
18	13.939	1851	1862	1875	rBV	887187	1236705	50.09%	6.052%
19	14.216	1902	1909	1923	rBV	959182	1363091	55.21%	6.670%
20	14.522	1954	1961	1969	rBV	632533	901187	36.50%	4.410%
21	14.751	1995	2000	2016	rBV	34781	74392	3.01%	0.364%
22	14.957	2032	2035	2040	rVB2	8078	9622	0.39%	0.047%
23	15.363	2099	2104	2107	rBV	4960	6054	0.25%	0.030%
24	15.516	2124	2130	2141	rVB	1294078	1796147	72.75%	8.790%
25	15.651	2147	2153	2166	rBV	258265	366518	14.85%	1.794%
26	15.757	2166	2171	2176	rVB3	6989	11027	0.45%	0.054%
27	15.922	2194	2199	2202	rBV4	1843	2733	0.11%	0.013%
28	16.222	2246	2250	2260	rBV	16554	28886	1.17%	0.141%
29	16.563	2300	2308	2312	rBV8	3117	6309	0.26%	0.031%
30	16.686	2324	2329	2332	rBV4	1847	3067	0.12%	0.015%
31	16.728	2332	2336	2343	rVB6	1641	3773	0.15%	0.018%
32	16.804	2343	2349	2351	rVB6	1512	3039	0.12%	0.015%
33	17.022	2381	2386	2390	rBV	11959	15695	0.64%	0.077%
34	17.069	2390	2394	2399	rVB6	5544	8355	0.34%	0.041%
35	17.275	2423	2429	2436	rBV	798858	1093660	44.30%	5.352%
36	17.375	2440	2446	2461	rVV2	1425903	2045446	82.85%	10.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022773.D
 Acq On : 19 Nov 2022 01:40
 Operator : CG/JU
 Sample : N5689-18
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

37	17.480	2461	2464	2468	rVB5	11561	15564	0.63%	0.076%
38	17.569	2474	2479	2482	rVB6	1731	2848	0.12%	0.014%
39	17.763	2508	2512	2516	rBV4	6299	8321	0.34%	0.041%
40	17.951	2541	2544	2549	rVB5	1989	3169	0.13%	0.016%
41	18.169	2576	2581	2588	rBV2	11314	18911	0.77%	0.093%
42	18.463	2627	2631	2638	rVB5	2666	4568	0.19%	0.022%
43	18.751	2676	2680	2683	rVB6	1724	2520	0.10%	0.012%
44	19.239	2760	2763	2768	rBV3	15595	20210	0.82%	0.099%
45	19.310	2771	2775	2782	rVV	13605	18682	0.76%	0.091%
46	19.451	2796	2799	2805	rBV4	9842	14195	0.57%	0.069%
47	19.598	2821	2824	2828	rBV2	4085	5072	0.21%	0.025%
48	19.680	2831	2838	2849	rBV	1718047	2309119	93.53%	11.300%
49	21.480	3138	3144	3153	rBV	936290	1212969	49.13%	5.936%
50	23.721	3517	3525	3536	rVB	1212219	2468919	100.00%	12.082%
51	23.874	3544	3551	3562	rVB2	619597	1225413	49.63%	5.997%




Sum of corrected areas: 20434740

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022773.D
Acq On : 19 Nov 2022 01:40
Operator : CG/JU
Sample : N5689-18
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

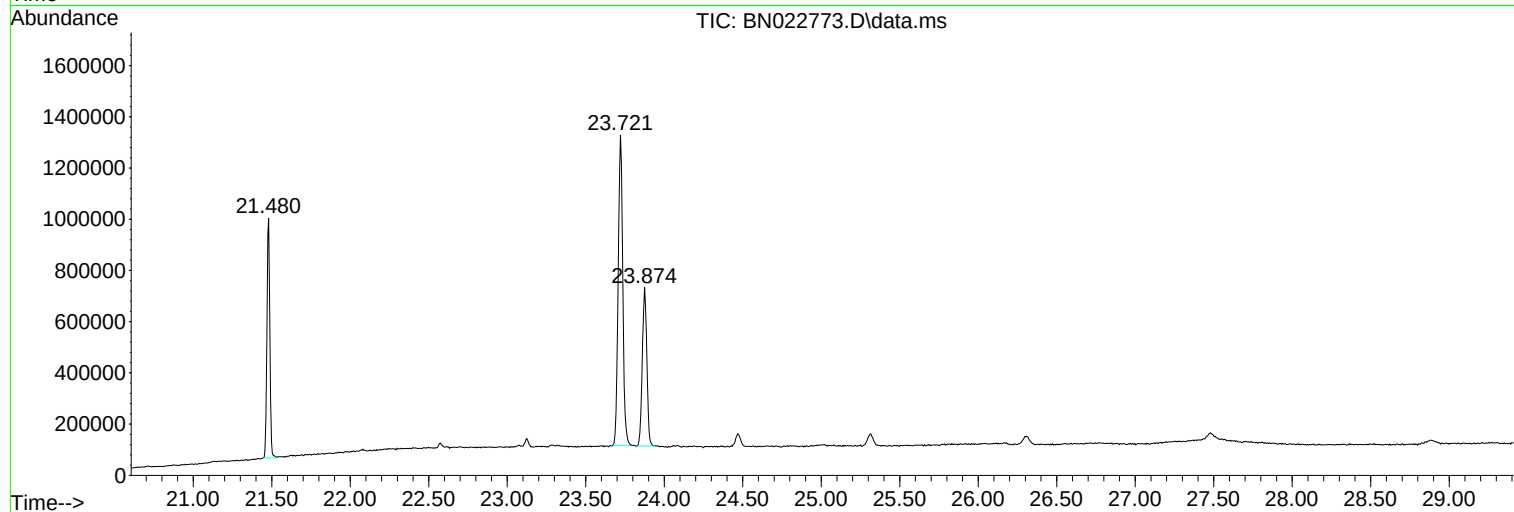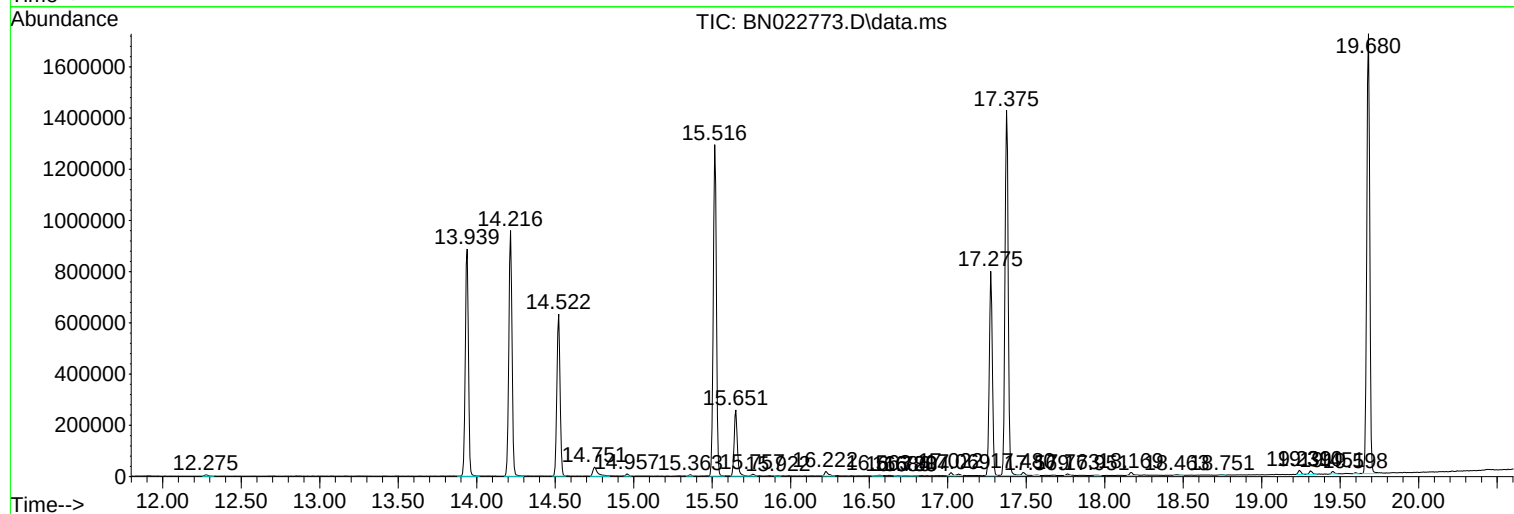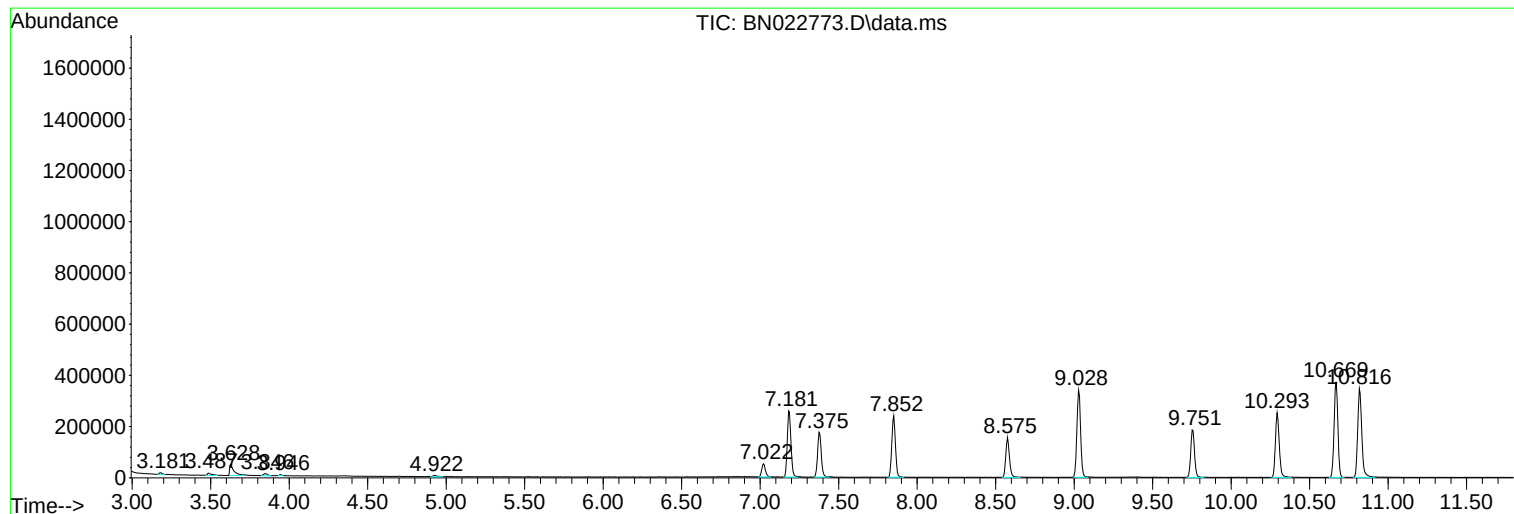

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022773.D
Acq On : 19 Nov 2022 01:40
Operator : CG/JU
Sample : N5689-18
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022773.D
Acq On : 19 Nov 2022 01:40
Operator : CG/JU
Sample : N5689-18
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc