

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
 Data File : BN022775.D
 Acq On : 19 Nov 2022 02:53
 Operator : CG/JU
 Sample : N5689-20
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGCG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	30	32	40	rVB	5104	7063	0.33%	0.042%
2	3.622	106	108	125	rBV	45987	92564	4.34%	0.551%
3	3.846	141	146	152	rVB2	5399	9572	0.45%	0.057%
4	3.946	159	163	168	rBV4	3399	5971	0.28%	0.036%
5	7.022	680	686	699	rVB	44842	76020	3.57%	0.453%
6	7.181	706	713	728	rBV	204739	327238	15.35%	1.949%
7	7.375	740	746	761	rVB	179183	297234	13.95%	1.771%
8	7.852	818	827	838	rBV	179185	290852	13.65%	1.733%
9	8.575	944	950	962	rBV	145734	239131	11.22%	1.425%
10	9.028	1020	1027	1039	rBV	268965	432603	20.30%	2.577%
11	9.404	1087	1091	1096	rVB4	1413	2913	0.14%	0.017%
12	9.751	1144	1150	1159	rBV	203199	338757	15.89%	2.018%
13	10.293	1235	1242	1259	rBV	272521	465190	21.83%	2.771%
14	10.669	1299	1306	1314	rVB	282621	469455	22.03%	2.797%
15	10.816	1321	1331	1348	rBV	268528	501512	23.53%	2.988%
16	12.275	1575	1579	1586	rVB	3099	6301	0.30%	0.038%
17	13.410	1767	1772	1779	rBV4	1723	3712	0.17%	0.022%
18	13.934	1855	1861	1875	rVB	688081	960141	45.05%	5.720%
19	14.216	1902	1909	1923	rBV	733492	1048834	49.21%	6.248%
20	14.522	1954	1961	1971	rVB	479829	684456	32.11%	4.078%
21	14.751	1995	2000	2014	rBV	33108	73105	3.43%	0.436%
22	14.957	2033	2035	2038	rVB3	2415	2245	0.11%	0.013%
23	15.516	2124	2130	2139	rVV	996786	1401812	65.77%	8.351%
24	15.651	2147	2153	2168	rVV	339558	482126	22.62%	2.872%
25	15.763	2168	2172	2176	rVB3	2538	3791	0.18%	0.023%
26	17.275	2423	2429	2437	rBV	595652	830278	38.96%	4.946%
27	17.375	2440	2446	2462	rVV	1232974	1703265	79.92%	10.147%
28	17.486	2462	2465	2467	rVB2	2487	2609	0.12%	0.016%
29	18.169	2577	2581	2587	rBV2	11821	15770	0.74%	0.094%
30	19.239	2759	2763	2771	rBV4	11032	17102	0.80%	0.102%
31	19.316	2771	2776	2780	rBV	10690	16064	0.75%	0.096%
32	19.451	2795	2799	2808	rBV6	11844	18185	0.85%	0.108%
33	19.598	2822	2824	2829	rBV5	1807	2981	0.14%	0.018%
34	19.680	2832	2838	2847	rBV	1457536	1917704	89.98%	11.424%
35	21.474	3138	3143	3151	rBV	717531	937933	44.01%	5.588%
36	23.715	3517	3524	3537	rVB2	1039165	2131306	100.00%	12.697%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION

37	23.874	3544	3551	3564	rVB2	479843	970161	45.52%	5.780%
----	--------	------	------	------	------	--------	--------	--------	--------




Sum of corrected areas: 16785956

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

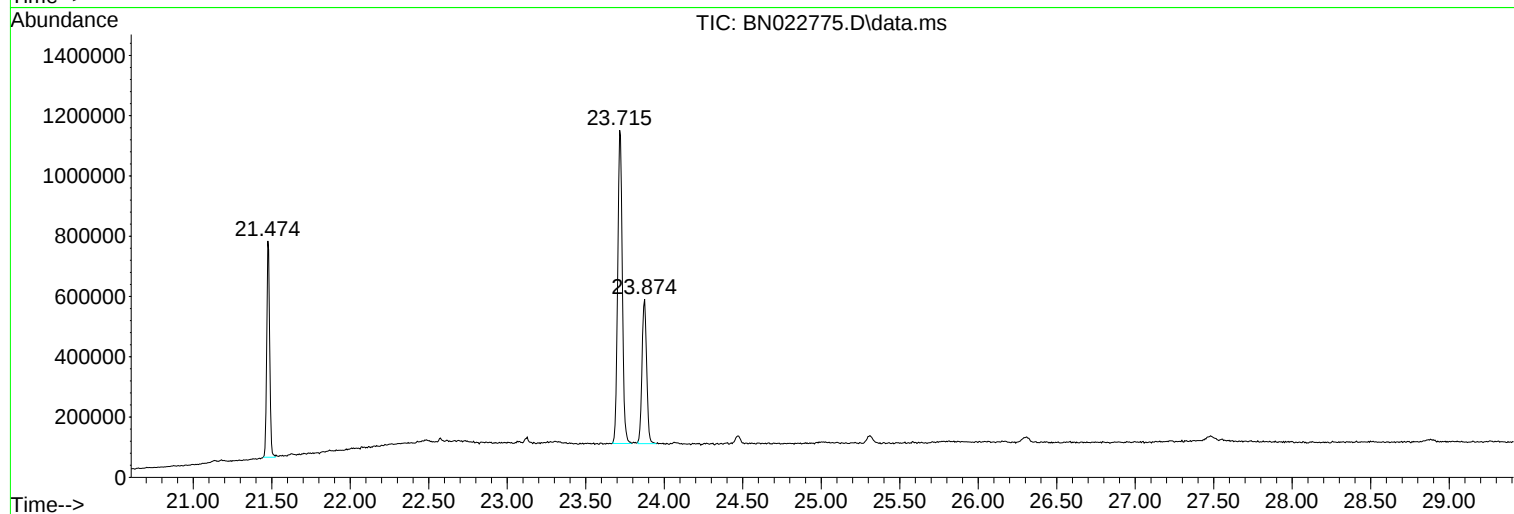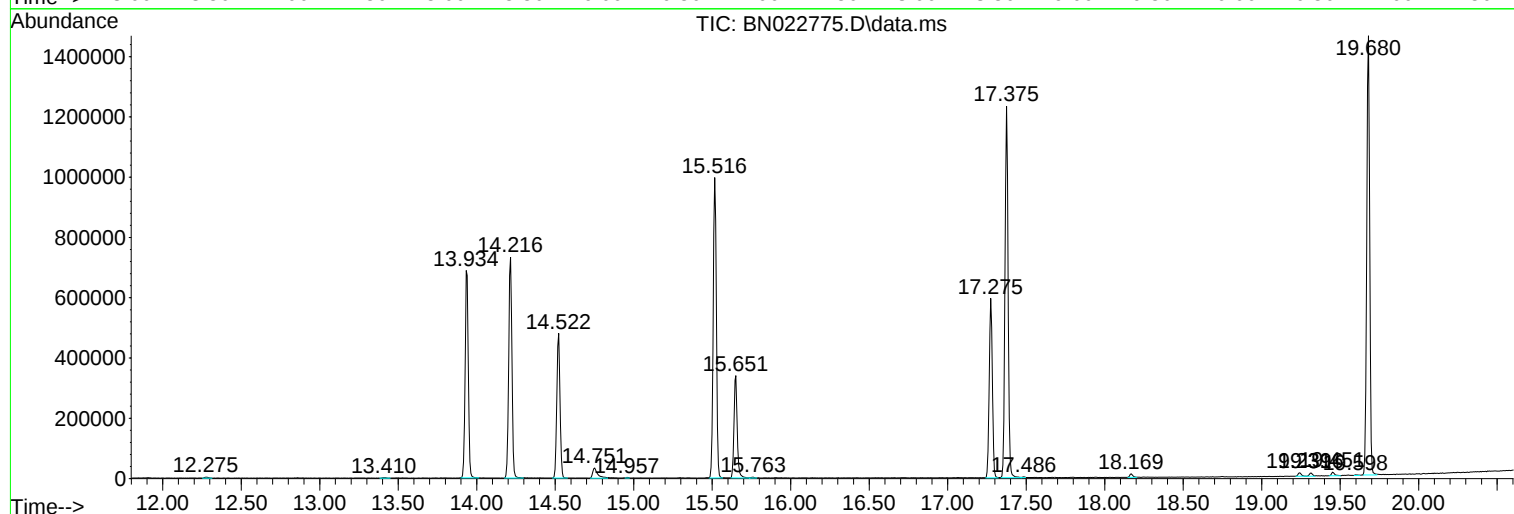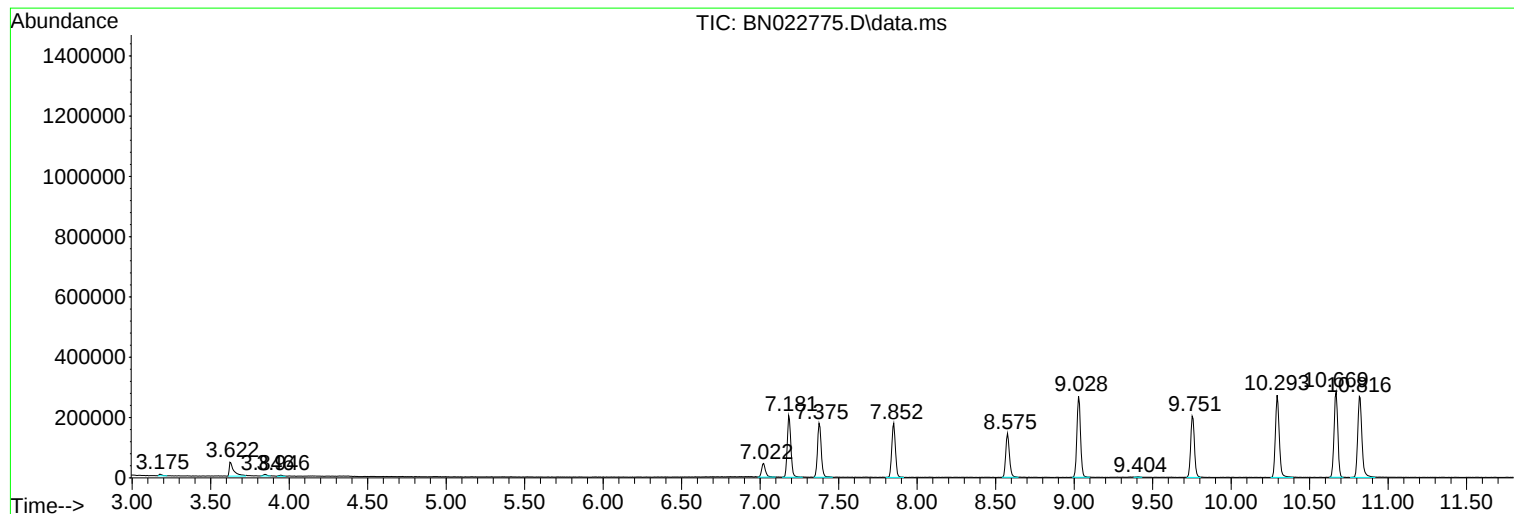

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111722\
Data File : BN022775.D
Acq On : 19 Nov 2022 02:53
Operator : CG/JU
Sample : N5689-20
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGCG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc