
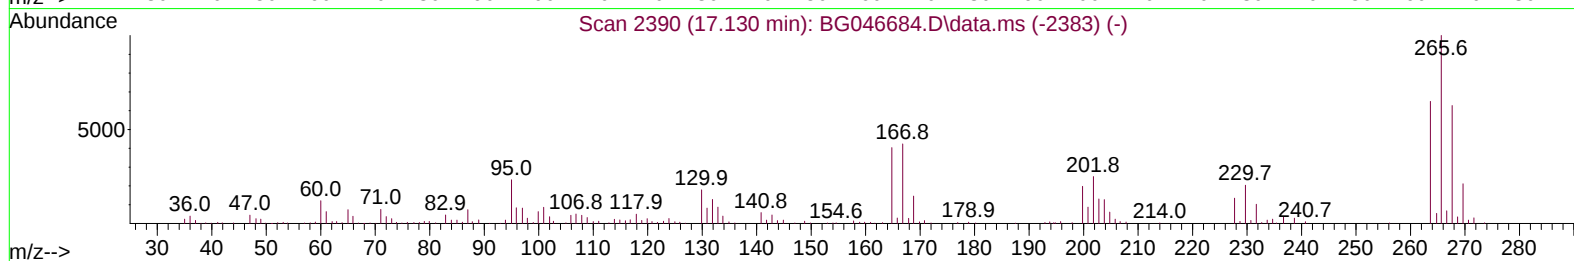
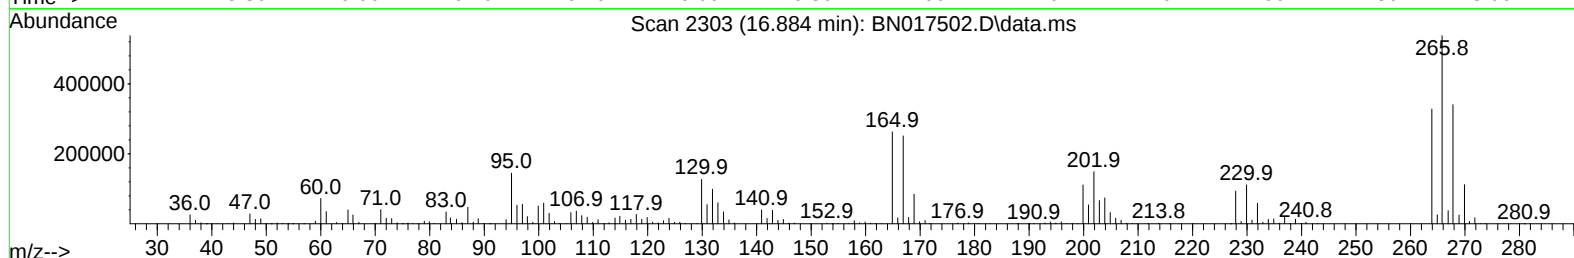


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111821\
Data File : BN017502.D
Acq On : 18 Nov 2021 08:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 09:52:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 18 09:51:37 2021
Response via : Initial Calibration

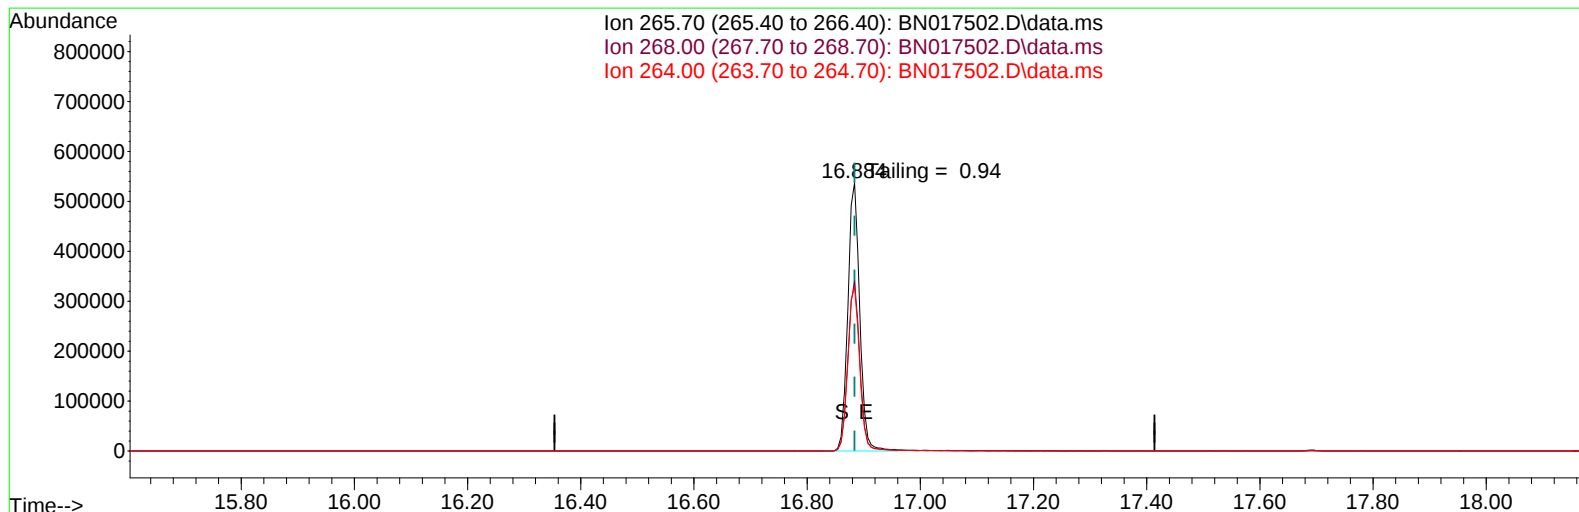

TIC: BN017502.D\data.ms

(70) Pentachlorophenol (C)




16.884min (0.000) 19295.12 ng

response 788915

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.36
264.00	61.60	61.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111821\
Data File : BN017502.D
Acq On : 18 Nov 2021 08:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 09:52:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 18 09:51:37 2021
Response via : Initial Calibration

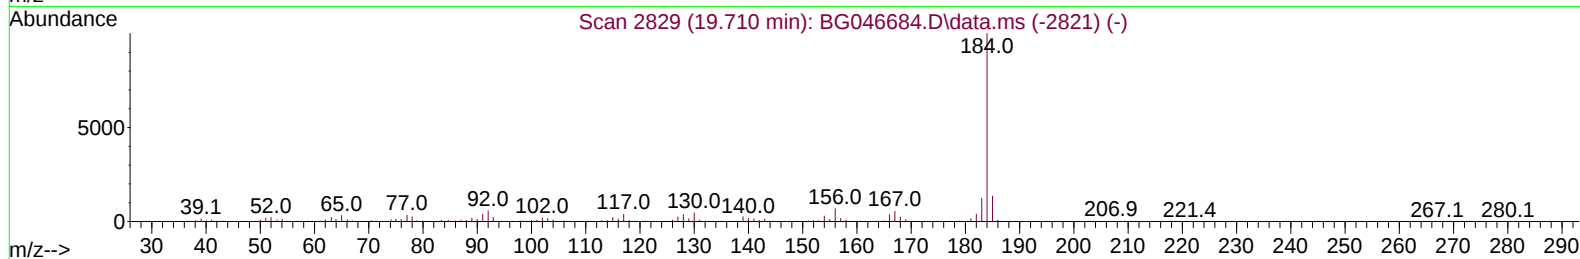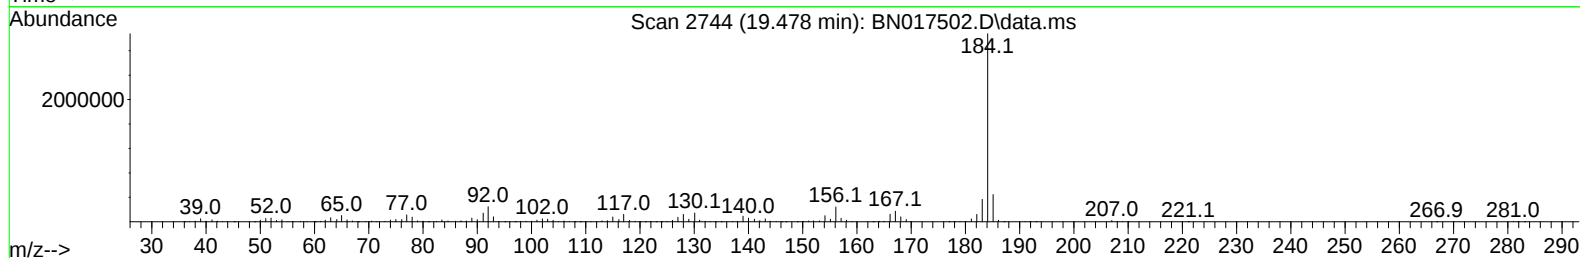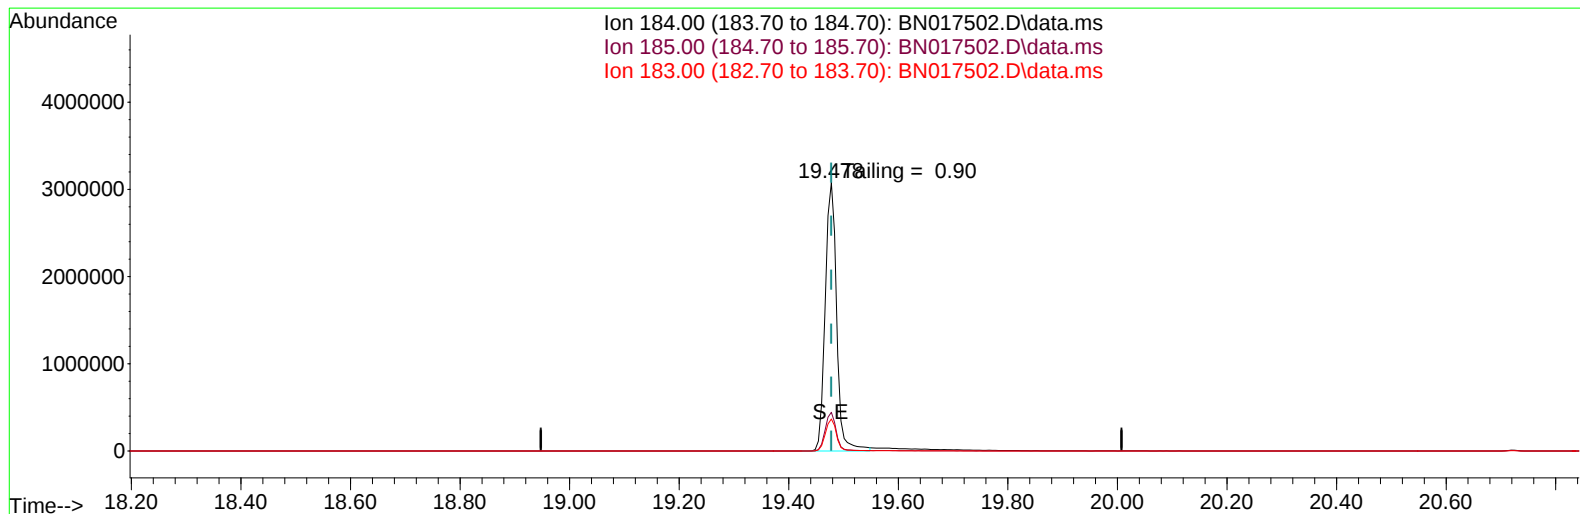

TIC: BN017502.D\data.ms

(77) Benzidine

19.478min (0.000) 0.00 ng

response 4715708

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	11.92
0.00	0.00	0.00