




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035151.D
Acq On : 18 Nov 2024 16:57
Operator : RC/JU
Sample : P4715-09DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 17:38:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

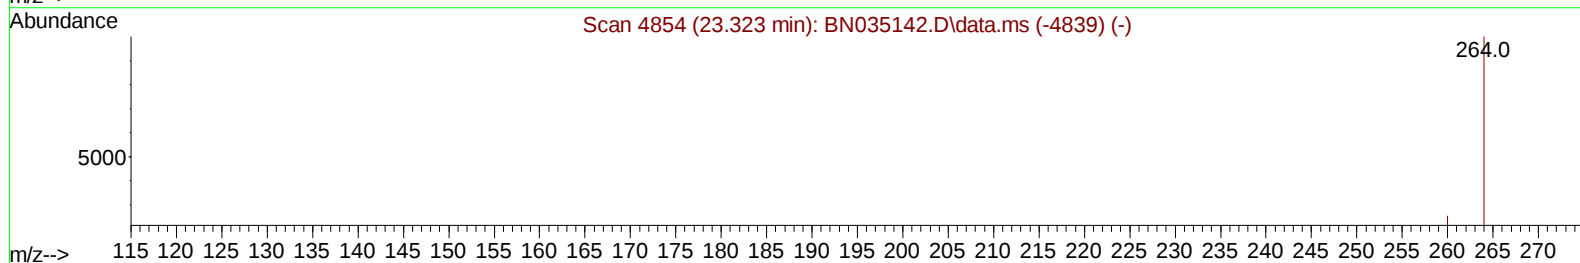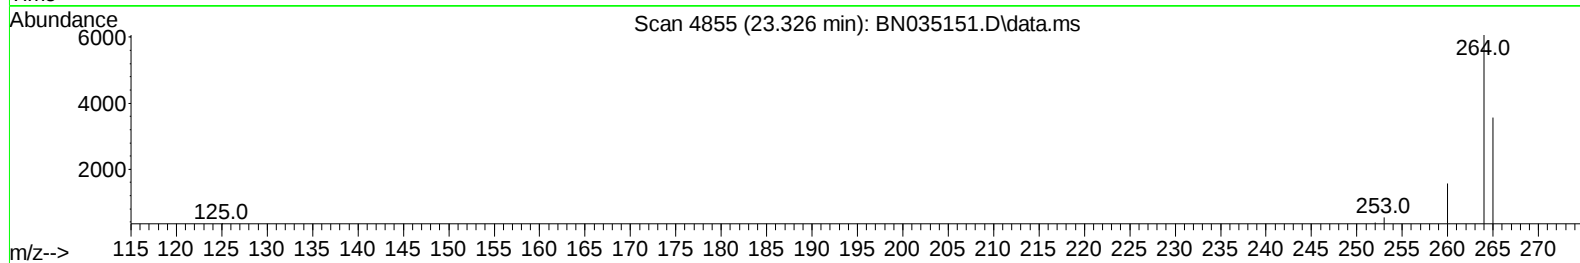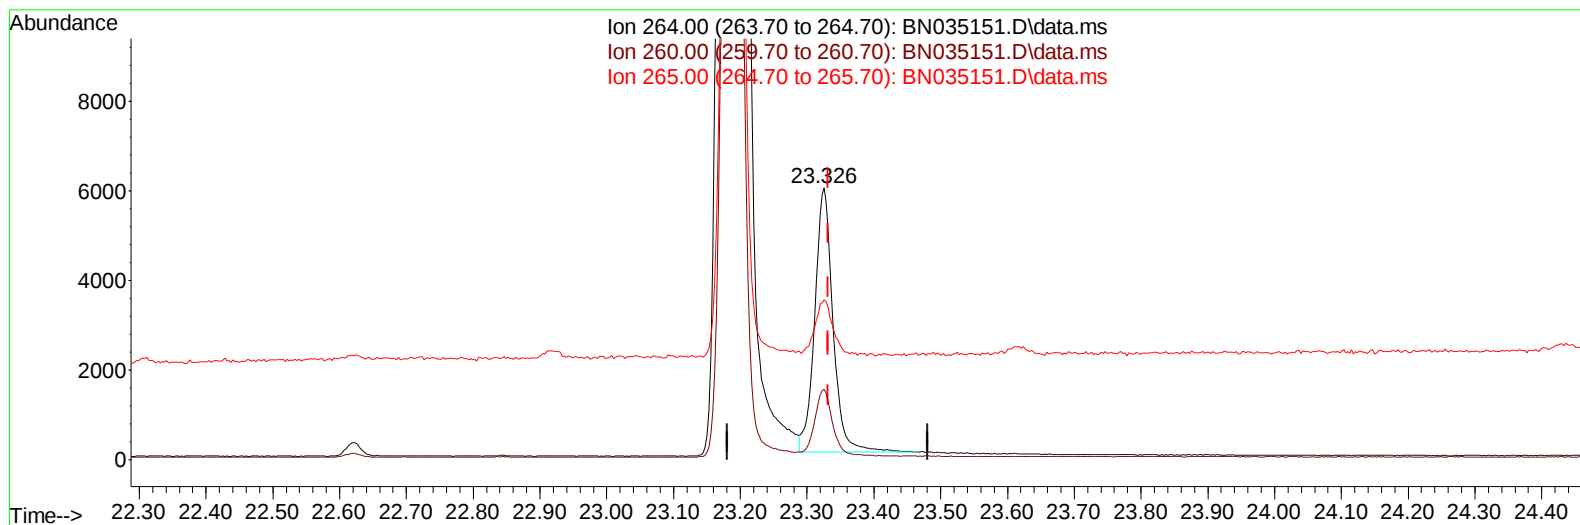

TIC: BN035151.D\data.ms

(23) Perylene-d12 (I)

23.326min (-0.006) 0.40 ng/u1

response 11266

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.88
265.00	75.50	58.95#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035151.D
Acq On : 18 Nov 2024 16:57
Operator : RC/JU
Sample : P4715-09DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 17:38:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

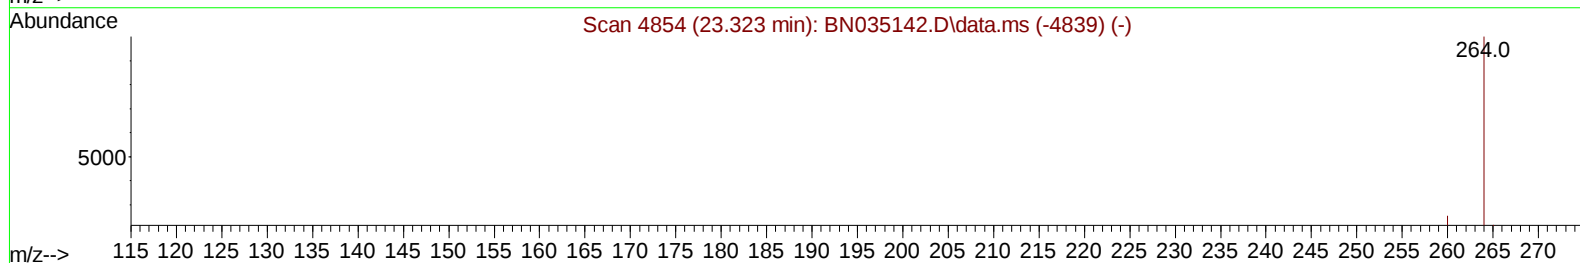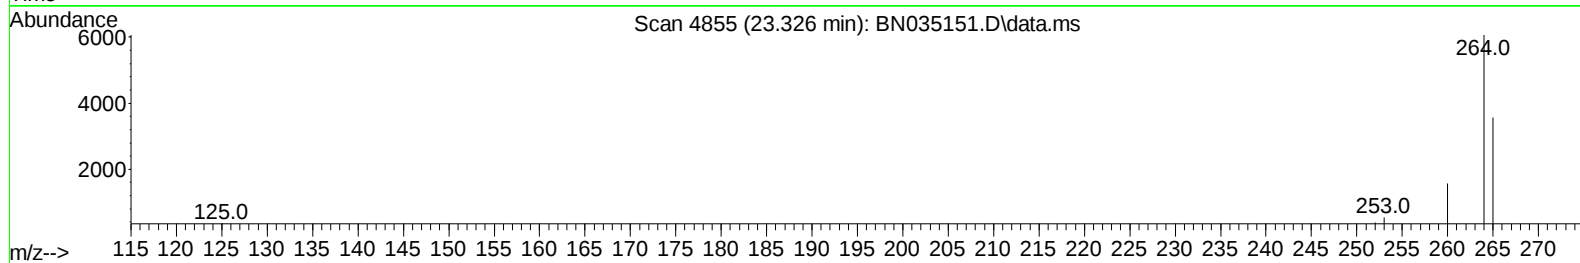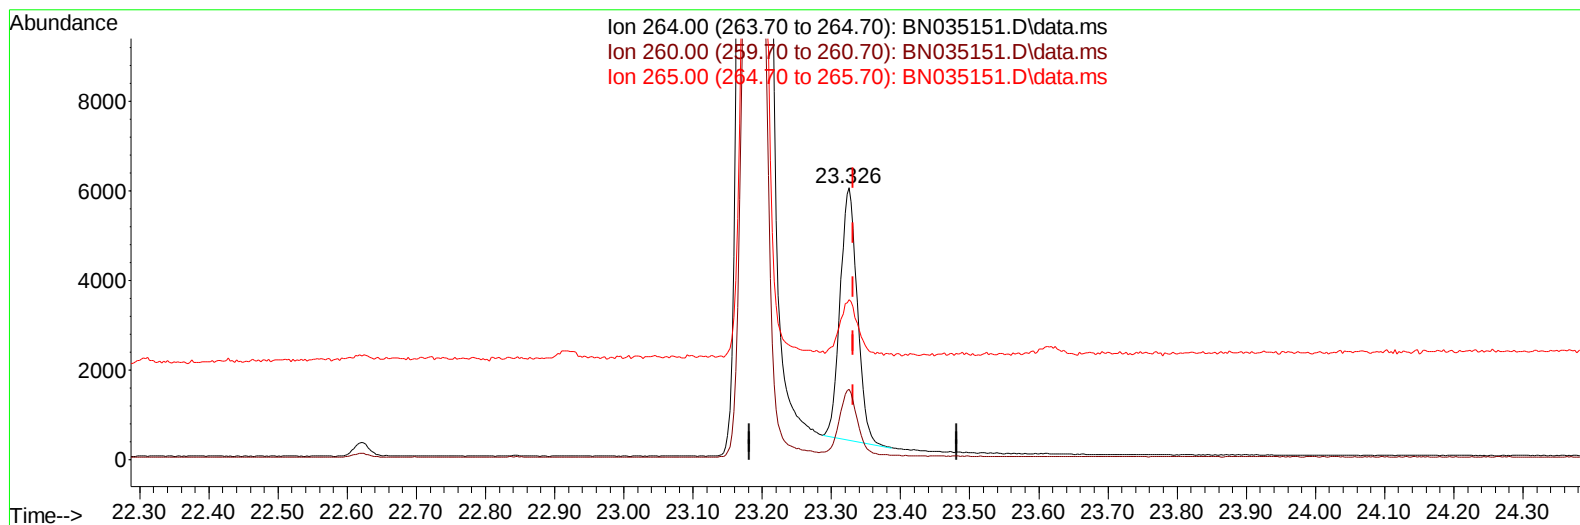

TIC: BN035151.D\data.ms

(23) Perylene-d12 (I)

23.326min (-0.006) 0.40 ng/ul m

response 9751

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.88
265.00	75.50	58.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
 Data File : BN035151.D
 Acq On : 18 Nov 2024 16:57
 Operator : RC/JU
 Sample : P4715-09DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AM0DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 18 17:38:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.545	152		2529	0.400	ng/ul	0.00
4) Naphthalene-d8	10.306	136		6038	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.189	164		4202	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188		9565	0.400	ng/ul	0.00
17) Chrysene-d12	21.151	240		9114	0.400	ng/ul	0.00
23) Perylene-d12	23.326	264		9751m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.140	96		3253	1.407	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.906	152		778	0.088	ng/ul	0.00
18) Fluoranthene-d10	18.981	212		2556	0.102	ng/ul	0.00
Target Compounds							
14) Pentachlorophenol	16.595	266		3453	1.550	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035151.D
Acq On : 18 Nov 2024 16:57
Operator : RC/JU
Sample : P4715-09DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 17:38:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

