




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035153.D
Acq On : 18 Nov 2024 18:09
Operator : RC/JU
Sample : SP6687
Misc : SFAM SURROGATE
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6687

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

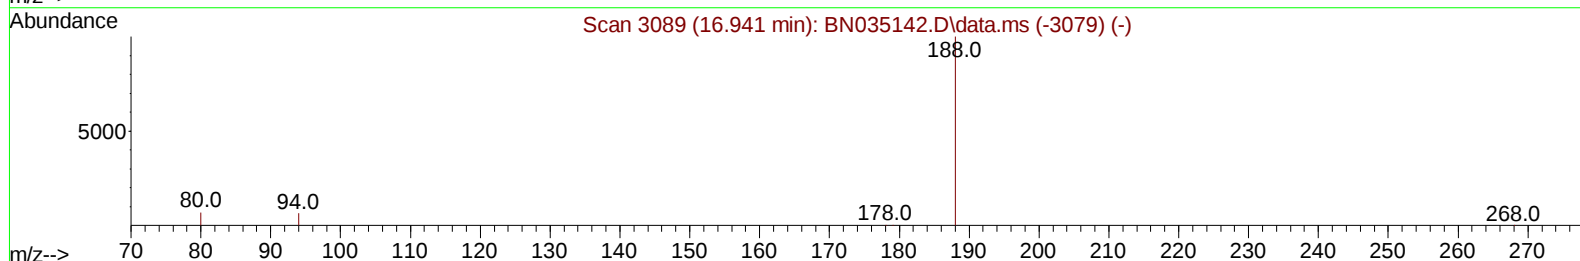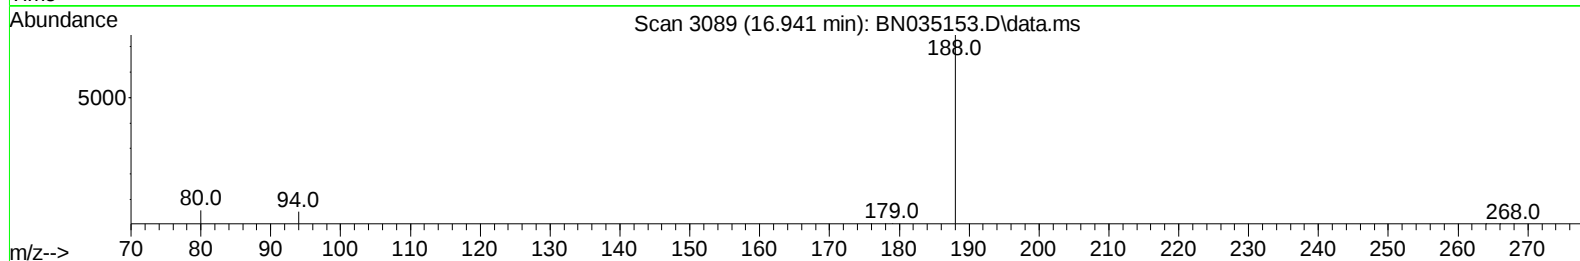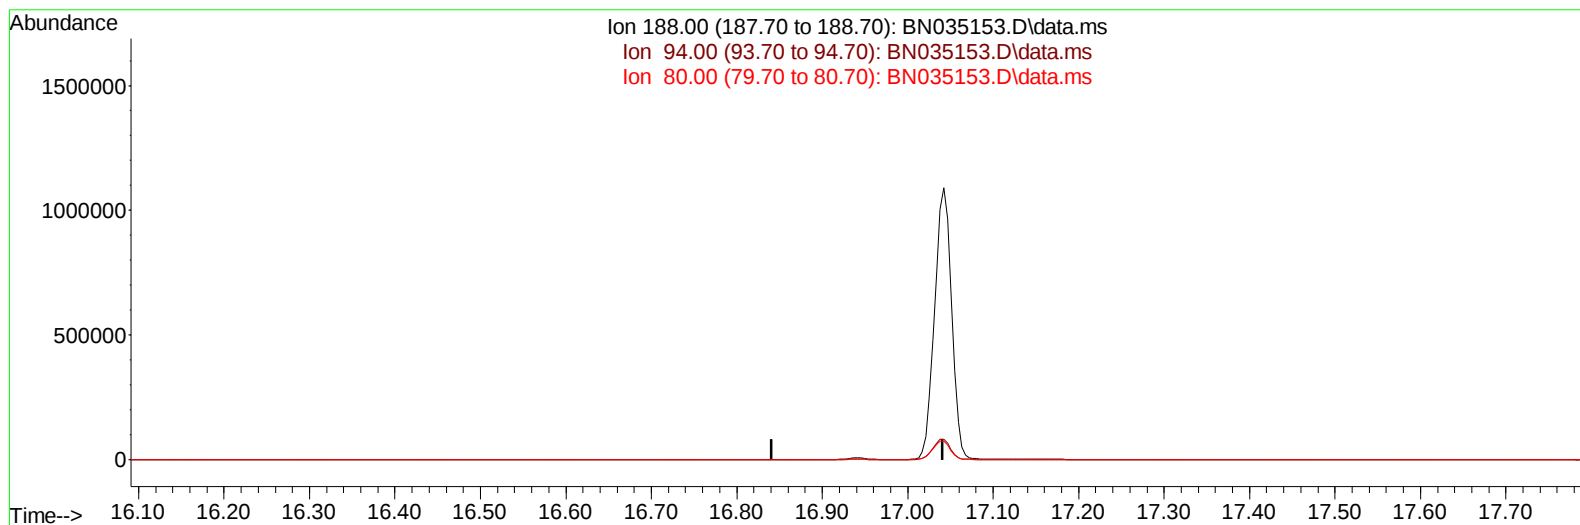

TIC: BN035153.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035153.D
Acq On : 18 Nov 2024 18:09
Operator : RC/JU
Sample : SP6687
Misc : SFAM SURROGATE
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6687

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

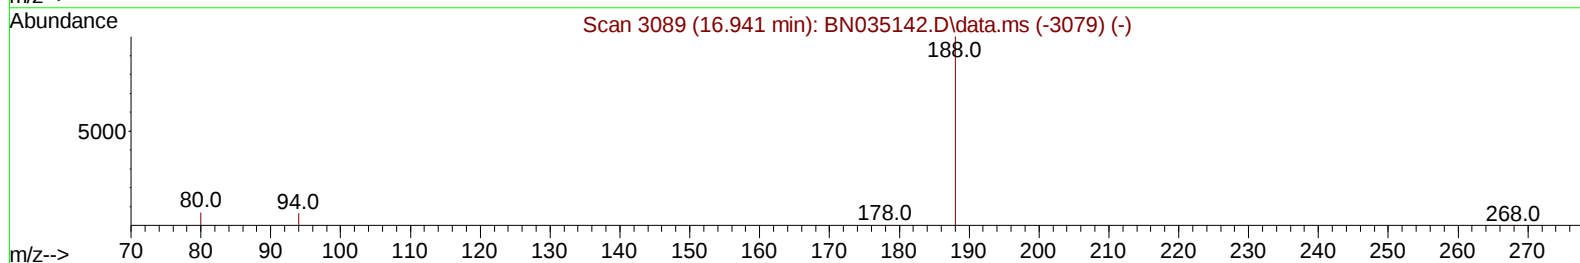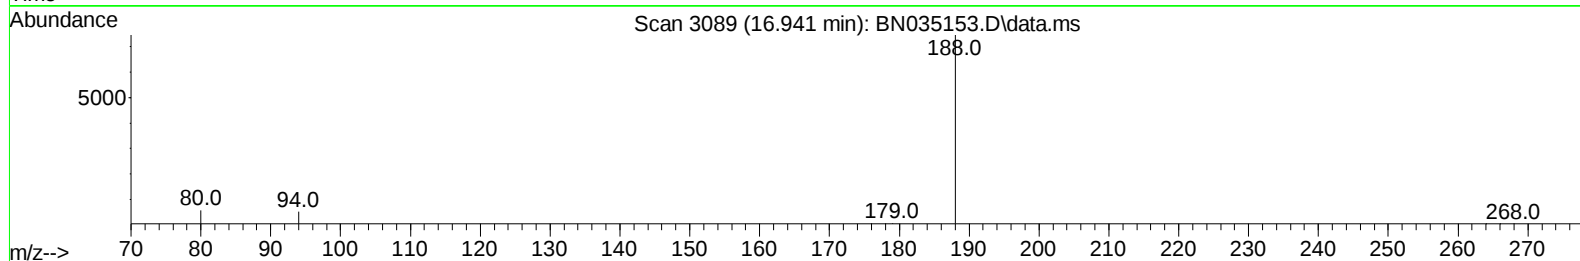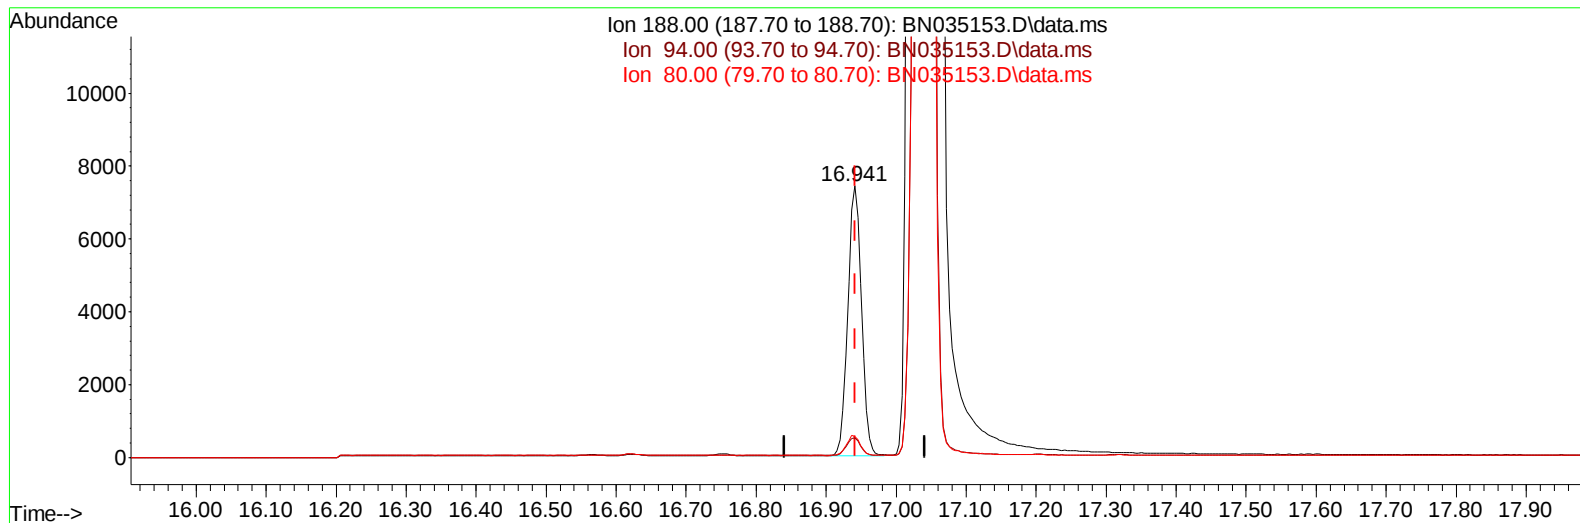

TIC: BN035153.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-0.000) 0.40 ng/ul m

response 10037

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	7.09
80.00	7.60	7.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
 Data File : BN035153.D
 Acq On : 18 Nov 2024 18:09
 Operator : RC/JU
 Sample : SP6687
 Misc : SFAM SURROGATE
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP6687

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

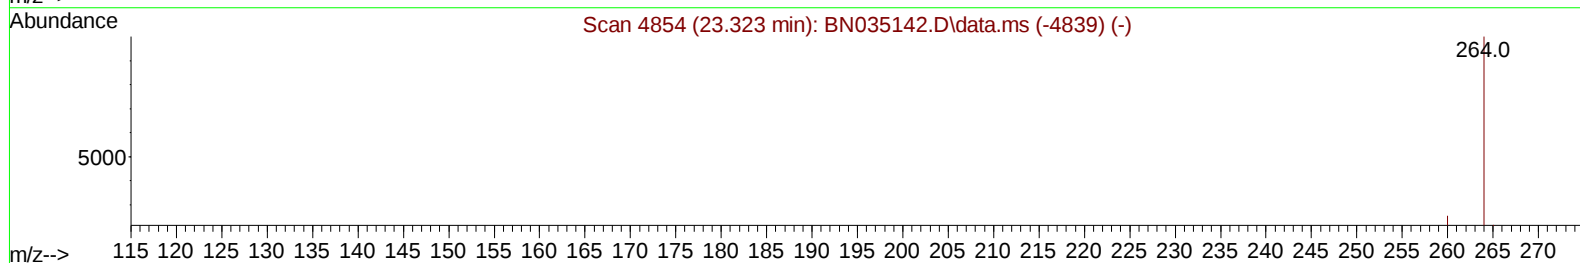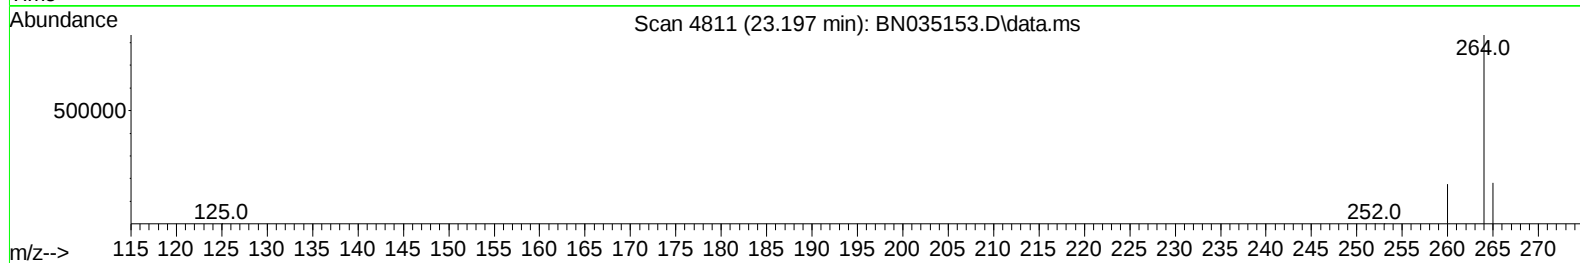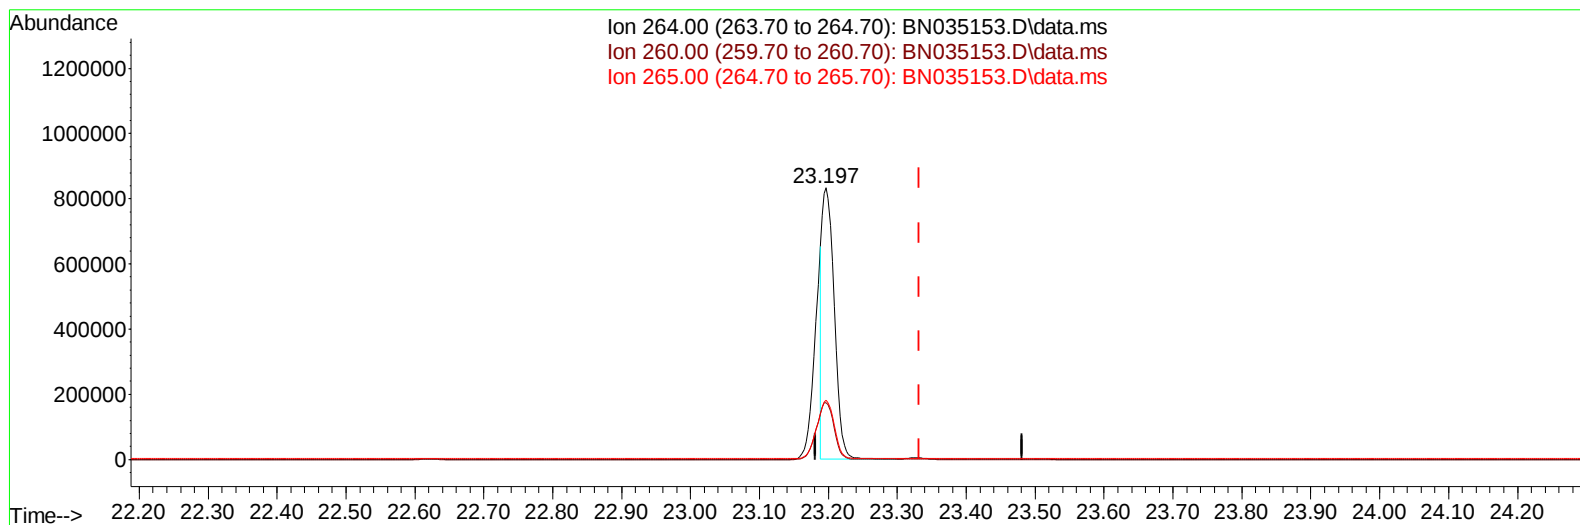

TIC: BN035153.D\data.ms

(23) Perylene-d12 (I)

23.197min (-0.135) 0.40 ng/u1

response 1028285

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	20.97
265.00	75.50	21.78#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035153.D
Acq On : 18 Nov 2024 18:09
Operator : RC/JU
Sample : SP6687
Misc : SFAM SURROGATE
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6687

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 18 22:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

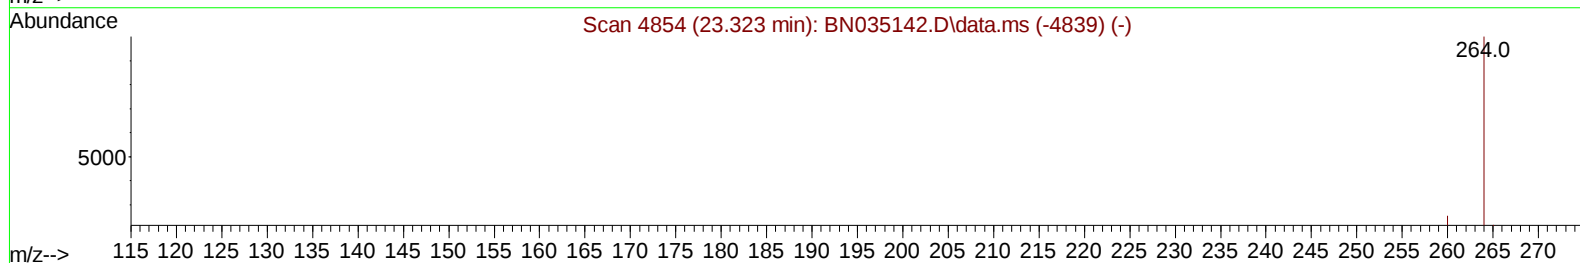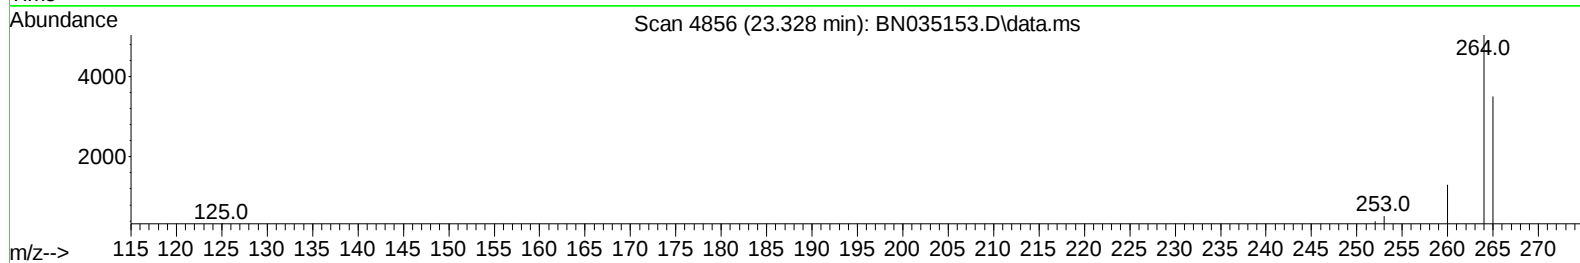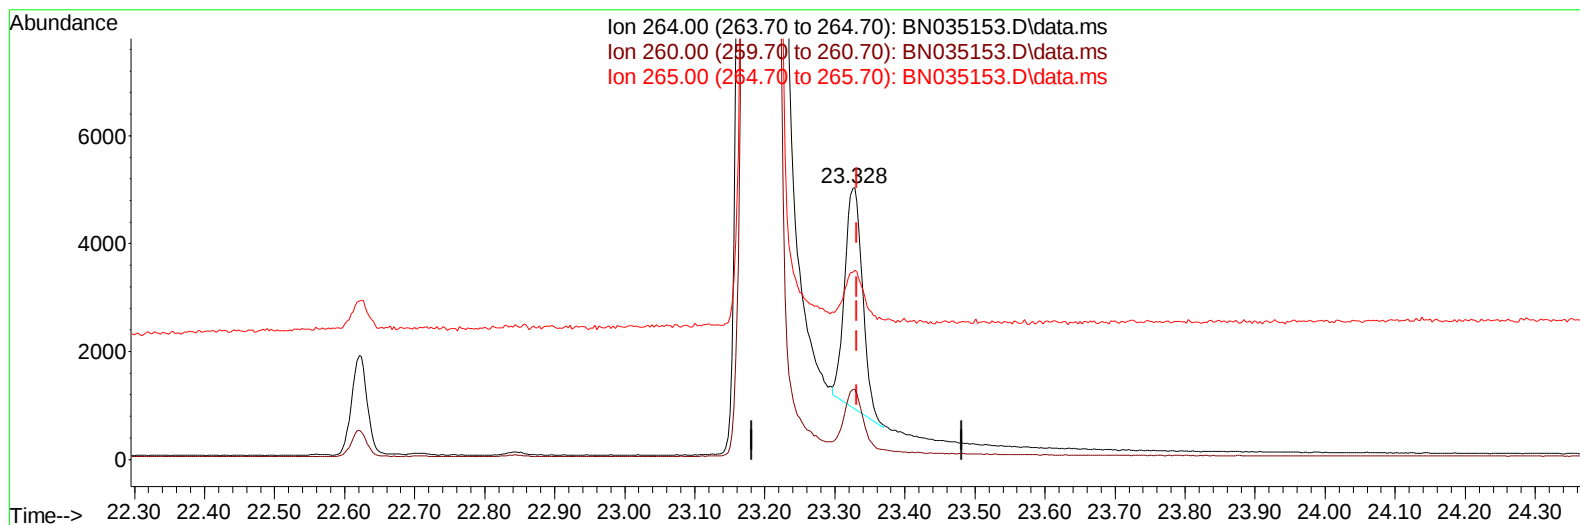

TIC: BN035153.D\data.ms

(23) Perylene-d12 (I)

23.328min (-0.003) 0.40 ng/ul m

response 7217

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.85
265.00	75.50	69.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
 Data File : BN035153.D
 Acq On : 18 Nov 2024 18:09
 Operator : RC/JU
 Sample : SP6687
 Misc : SFAM SURROGATE
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP6687

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 18 22:26:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.554	152	2498	0.400	ng/ul	0.00
4) Naphthalene-d8	10.311	136	6047	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.185	164	4436	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	10037m	0.400	ng/ul	0.00
17) Chrysene-d12	21.154	240	7963	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	7217m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.186	96	35428	15.517	ng/ul	0.05
6) 2-Methylnaphthalene-d10	11.906	152	7132	0.805	ng/ul	0.00
18) Fluoranthene-d10	18.981	212	18813	0.856	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035153.D
Acq On : 18 Nov 2024 18:09
Operator : RC/JU
Sample : SP6687
Misc : SFAM SURROGATE
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6687

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

