




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035154.D
Acq On : 18 Nov 2024 18:45
Operator : RC/JU
Sample : SP6688
Misc : SFAM SIM SURROGATE
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6688

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

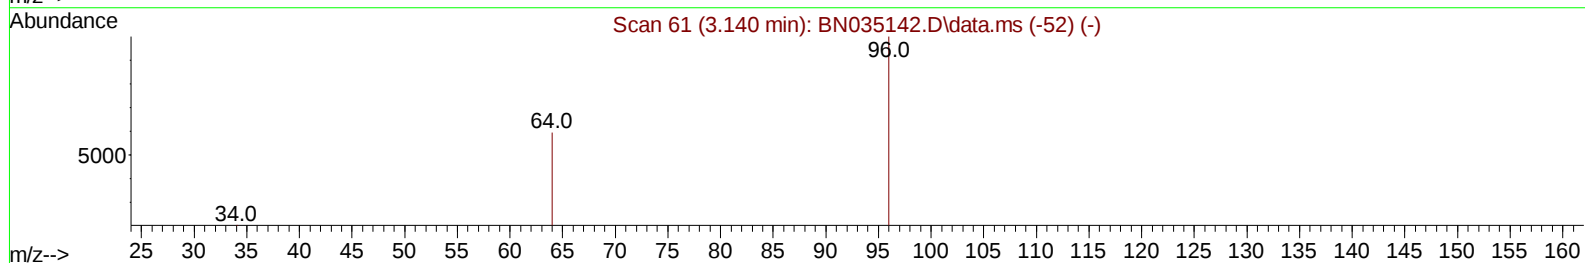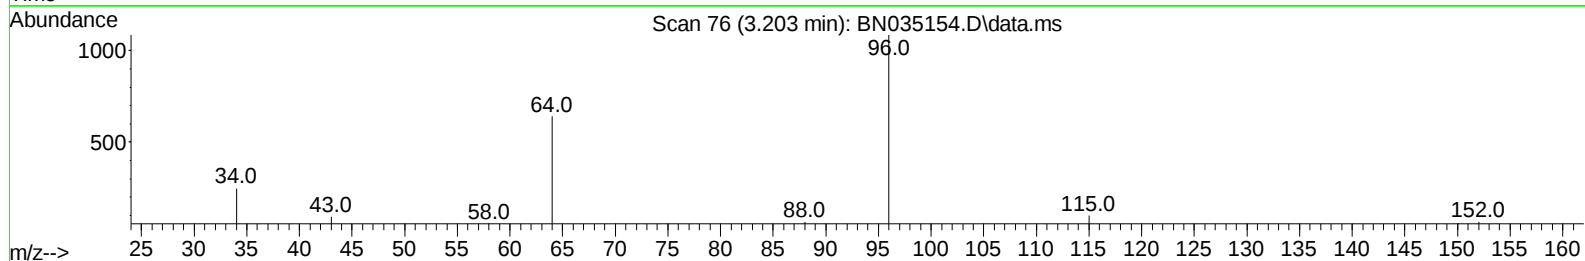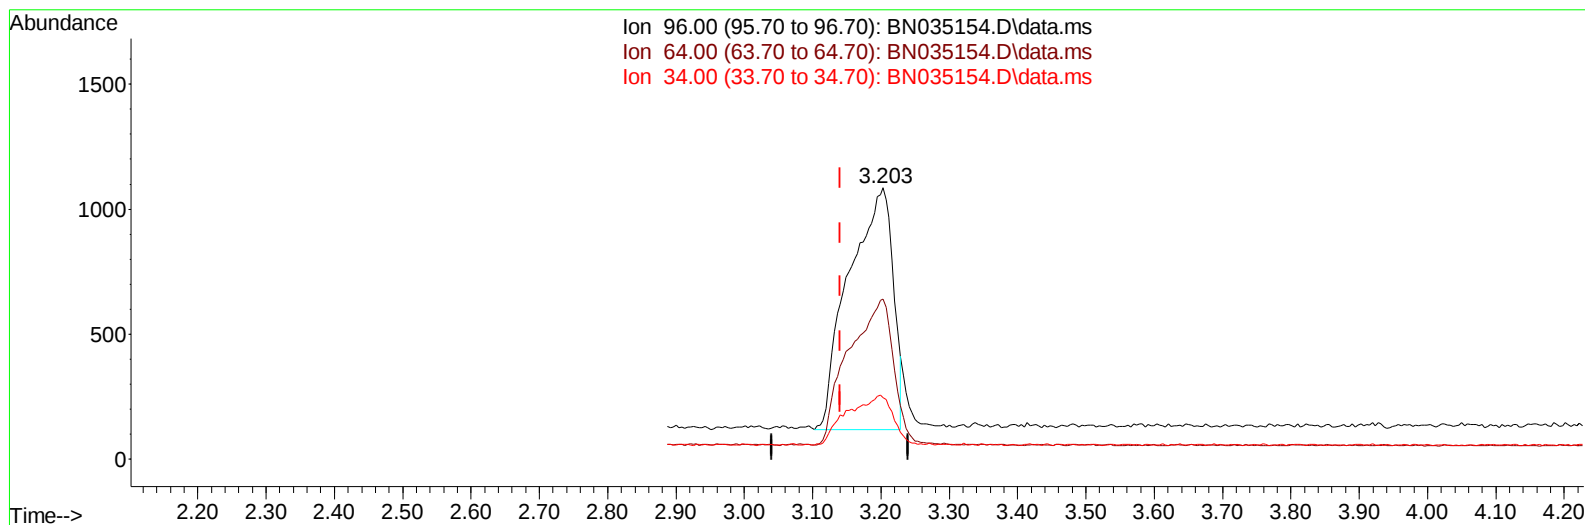

TIC: BN035154.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.203min (+ 0.063) 1.88 ng/u1

response 4317

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.00	58.99
34.00	26.30	22.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035154.D
Acq On : 18 Nov 2024 18:45
Operator : RC/JU
Sample : SP6688
Misc : SFAM SIM SURROGATE
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6688

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

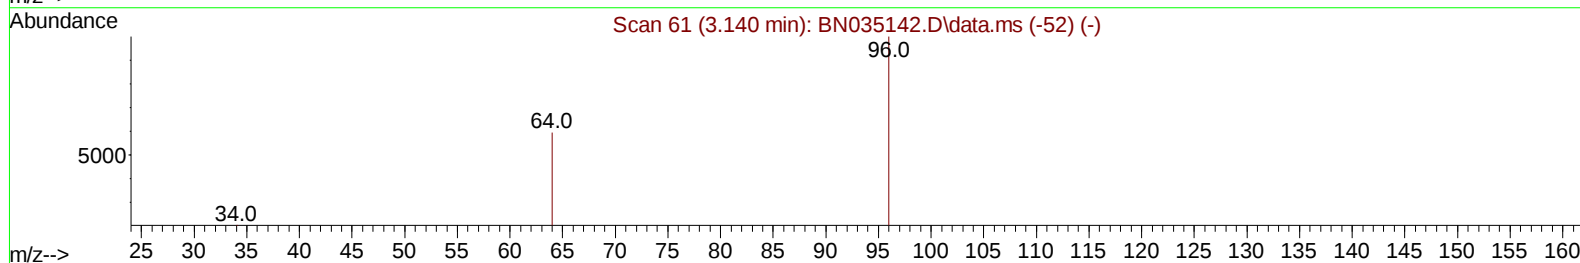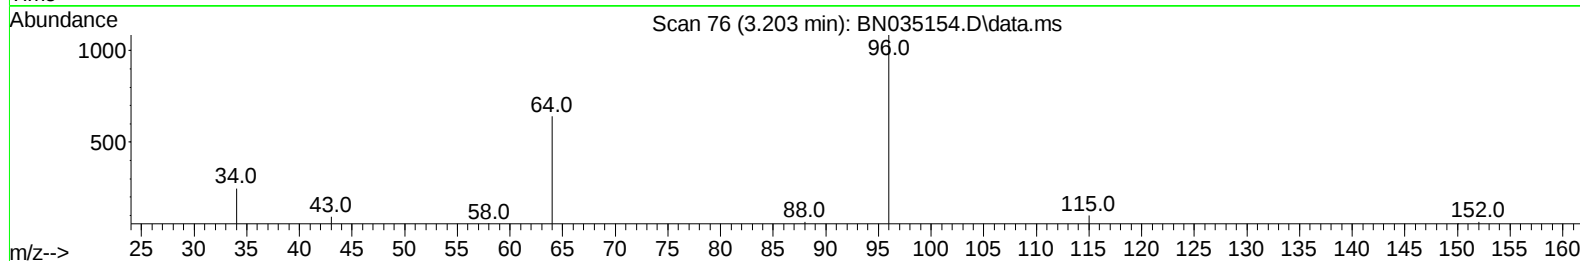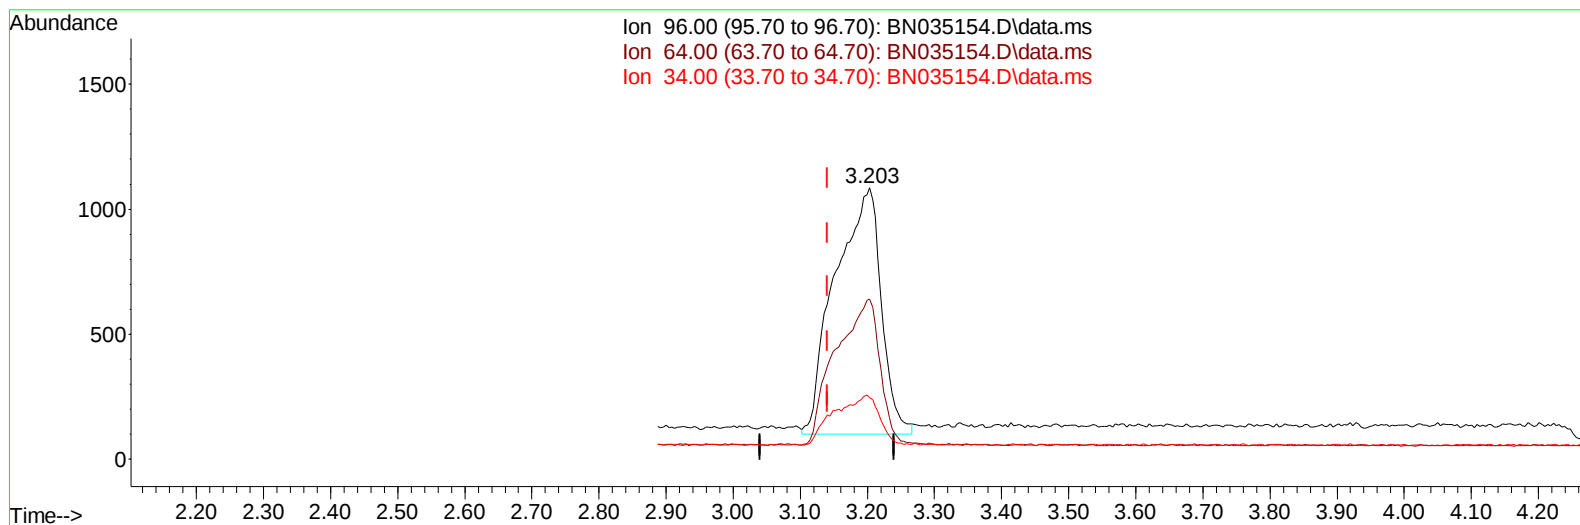

TIC: BN035154.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.203min (+ 0.063) 2.04 ng/ul m

response 4672

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	62.00	58.99
34.00	26.30	22.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
 Data File : BN035154.D
 Acq On : 18 Nov 2024 18:45
 Operator : RC/JU
 Sample : SP6688
 Misc : SFAM SIM SURROGATE
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP6688

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 18 22:26:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	2506	0.400	ng/ul	0.00
4) Naphthalene-d8	10.311	136	5754	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.189	164	3708	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	7709	0.400	ng/ul	0.00
17) Chrysene-d12	21.151	240	5689	0.400	ng/ul	0.00
23) Perylene-d12	23.325	264	5686	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.203	96	4672m	2.040	ng/ul	0.06
6) 2-Methylnaphthalene-d10	11.906	152	8043	0.954	ng/ul	0.00
18) Fluoranthene-d10	18.977	212	16647	1.061	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035154.D
Acq On : 18 Nov 2024 18:45
Operator : RC/JU
Sample : SP6688
Misc : SFAM SIM SURROGATE
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP6688

Manual IntegrationsAPPROVED

Quant Time: Nov 18 22:26:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

