

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
 Data File : BN035144.D
 Acq On : 18 Nov 2024 12:14
 Operator : RC/JU
 Sample : P4715-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAM0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/19/2024

Quant Time: Nov 18 12:38:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 00:44:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.545	152	3448	0.400	ng/u1	0.00
4) Naphthalene-d8	10.306	136	8488	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.189	164	5797	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.941	188	12966m	0.400	ng/u1	0.00
17) Chrysene-d12	21.154	240	11210	0.400	ng/u1	0.00
23) Perylene-d12	23.329	264	11428m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.136	96	17709	5.619	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.906	152	4295	0.345	ng/u1	0.00
18) Fluoranthene-d10	18.981	212	13077	0.423	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.595	266	22201	7.351	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111824\
Data File : BN035144.D
Acq On : 18 Nov 2024 12:14
Operator : RC/JU
Sample : P4715-09
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
COAM0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024


Quant Time: Nov 18 12:38:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 00:44:37 2024
Response via : Initial Calibration

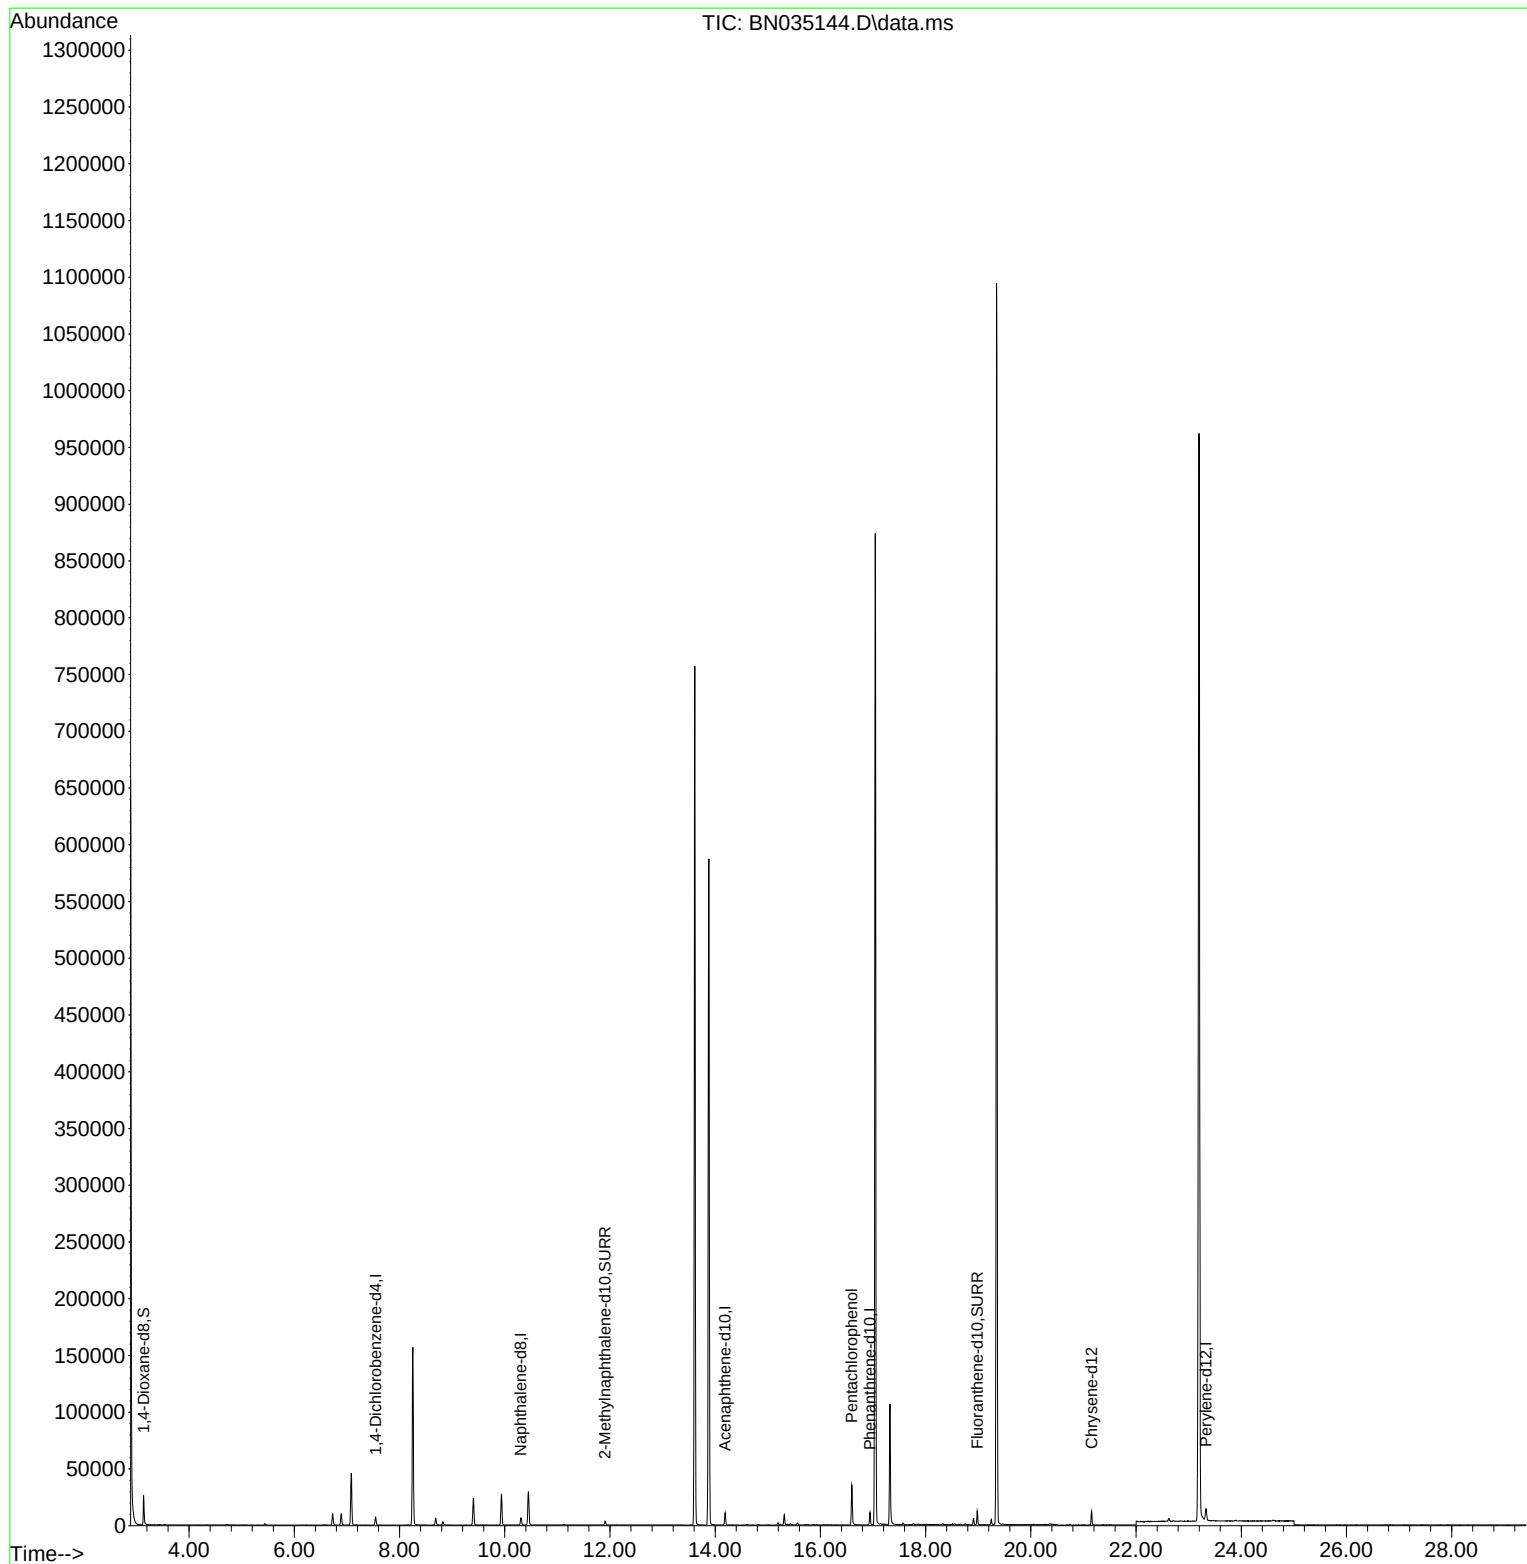

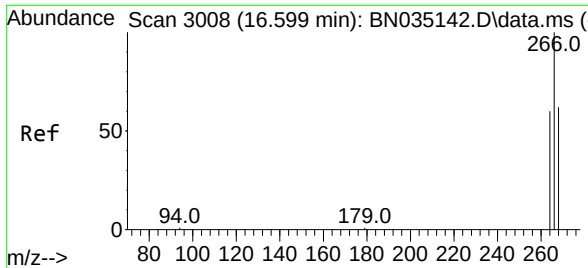

#14
Pentachlorophenol
Concen: 7.351 ng/ul
RT: 16.595 min Scan# 3007
Delta R.T. -0.004 min
Lab File: BN035144.D
Acq: 18 Nov 2024 12:14

Instrument :
BNA_N
ClientSampleId :
COAM0

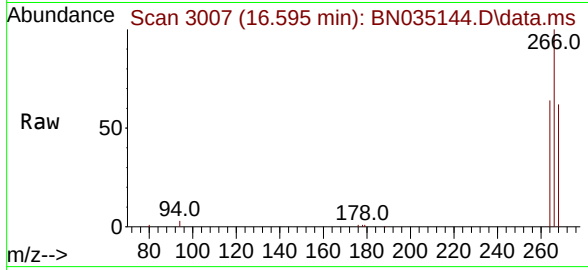

Tgt Ion:266 Resp: 2220
Ion Ratio Lower Upper
266 100
264 62.8 51.8 77.6
268 63.8 51.3 76.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/19/2024

