

Data File : BN003598.D
 Acq On : 19 Nov 2018 17:31
 Operator : MJ/SJ
 Sample : PB114864BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK64

Quant Time: Nov 20 01:49:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 20 01:46:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7521	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	26194	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	15985	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	3353725	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	43966	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	17081	0.42	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.47	166	5798	0.079	ng/ul#	11
23) Benzo(a)pyrene	23.56	252	16062	0.102	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003598.D
Acq On : 19 Nov 2018 17:31
Operator : MJ/SJ
Sample : PB114864BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK64

Quant Time: Nov 20 01:49:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration




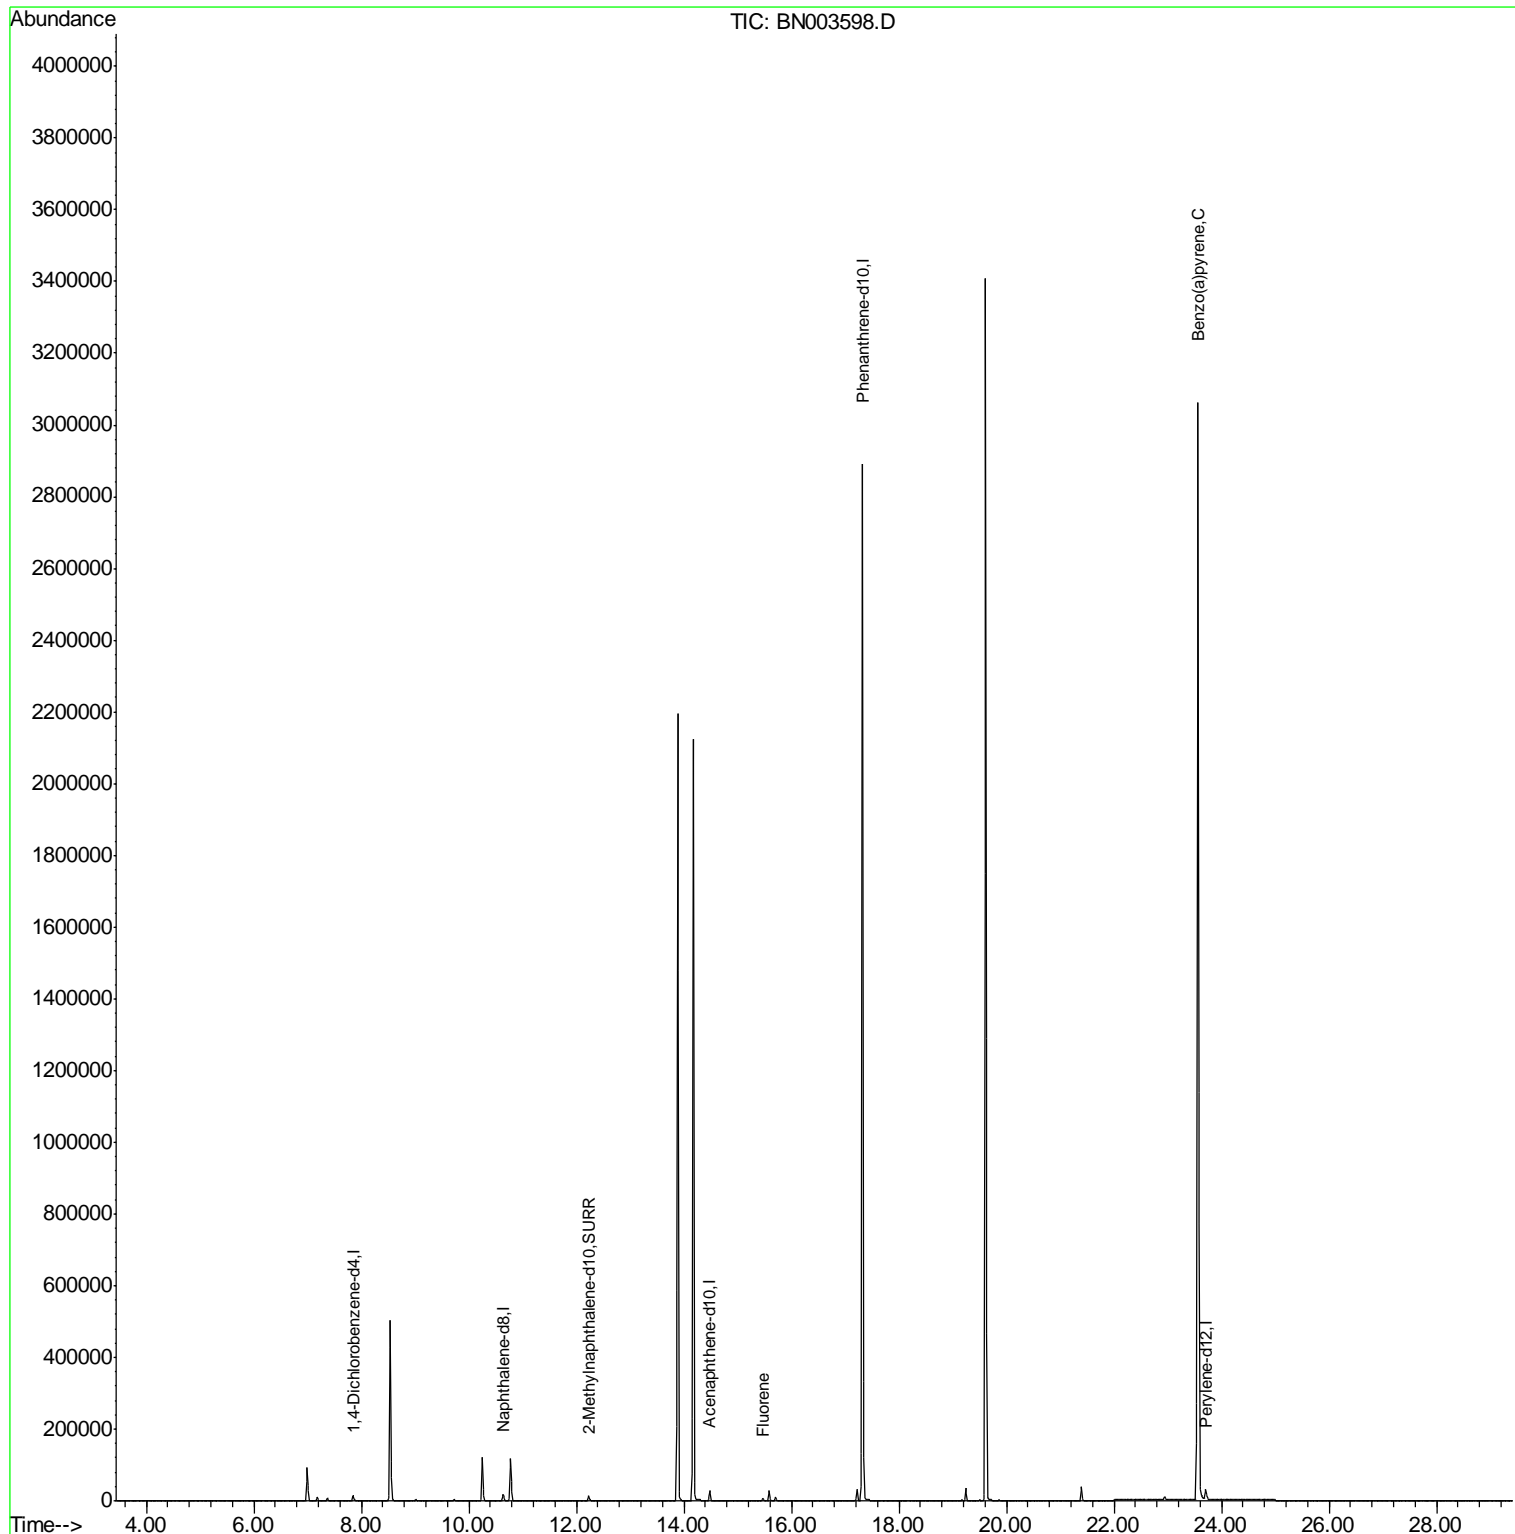


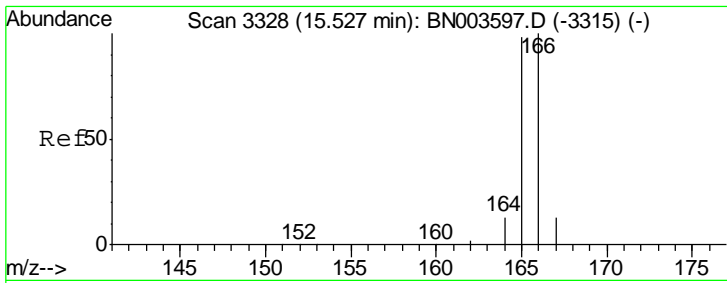

#9
 Fluorene
 Concen: 0.079 ng/ul
 RT: 15.47 min Scan# 3316
 Delta R.T. -0.06 min
 Lab File: BN003598.D
 Acq: 19 Nov 2018 17:31

Instrument :
 BNA_N
 ClientSampleID :
 SBLK64

Tgt Ion	Resp	Lower	Upper
166	5798		
165	4.4	78.3	117.5#
167	33.3	11.3	16.9#

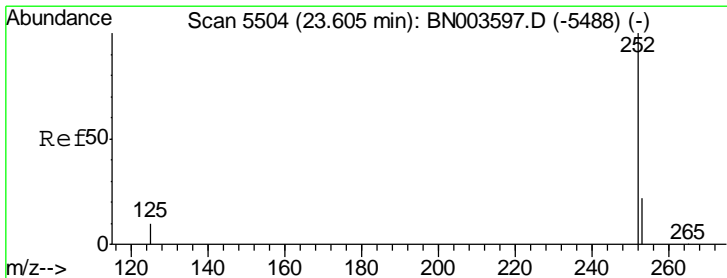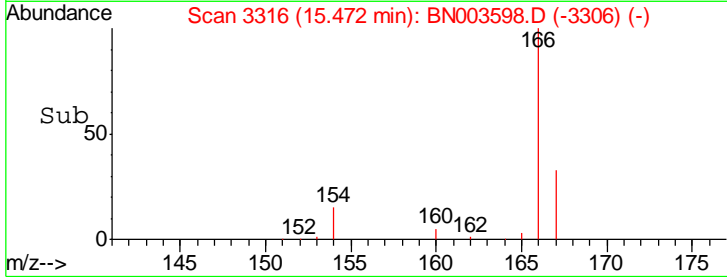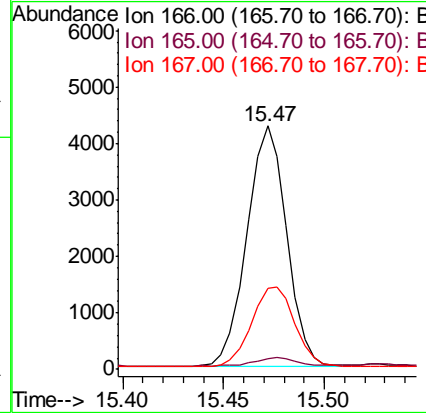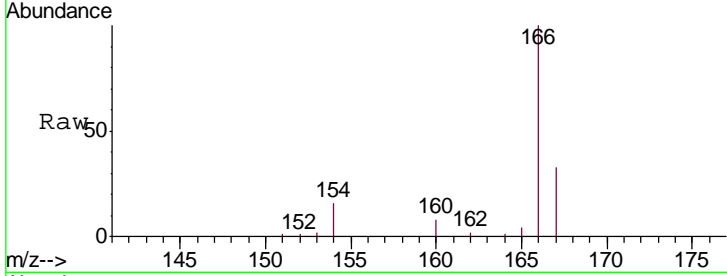

#23
 Benzo(a)pyrene
 Concen: 0.102 ng/ul
 RT: 23.56 min Scan# 5490
 Delta R.T. -0.04 min
 Lab File: BN003598.D
 Acq: 19 Nov 2018 17:31

Tgt Ion	Resp	Lower	Upper
252	16062		
253	30.3	19.0	28.4#
125	22.1	10.2	15.4#

