

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Not Reviewed)

Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z4

Quant Time: Nov 20 01:49:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	7196	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	31132	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	16537	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	1392442	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	47472	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	7071	0.15	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.56	252	6635	0.039	ng/ul#	Qvalue 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003601.D
Acq On : 19 Nov 2018 19:16
Operator : MJ/SJ
Sample : J5928-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z4

Quant Time: Nov 20 01:49:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

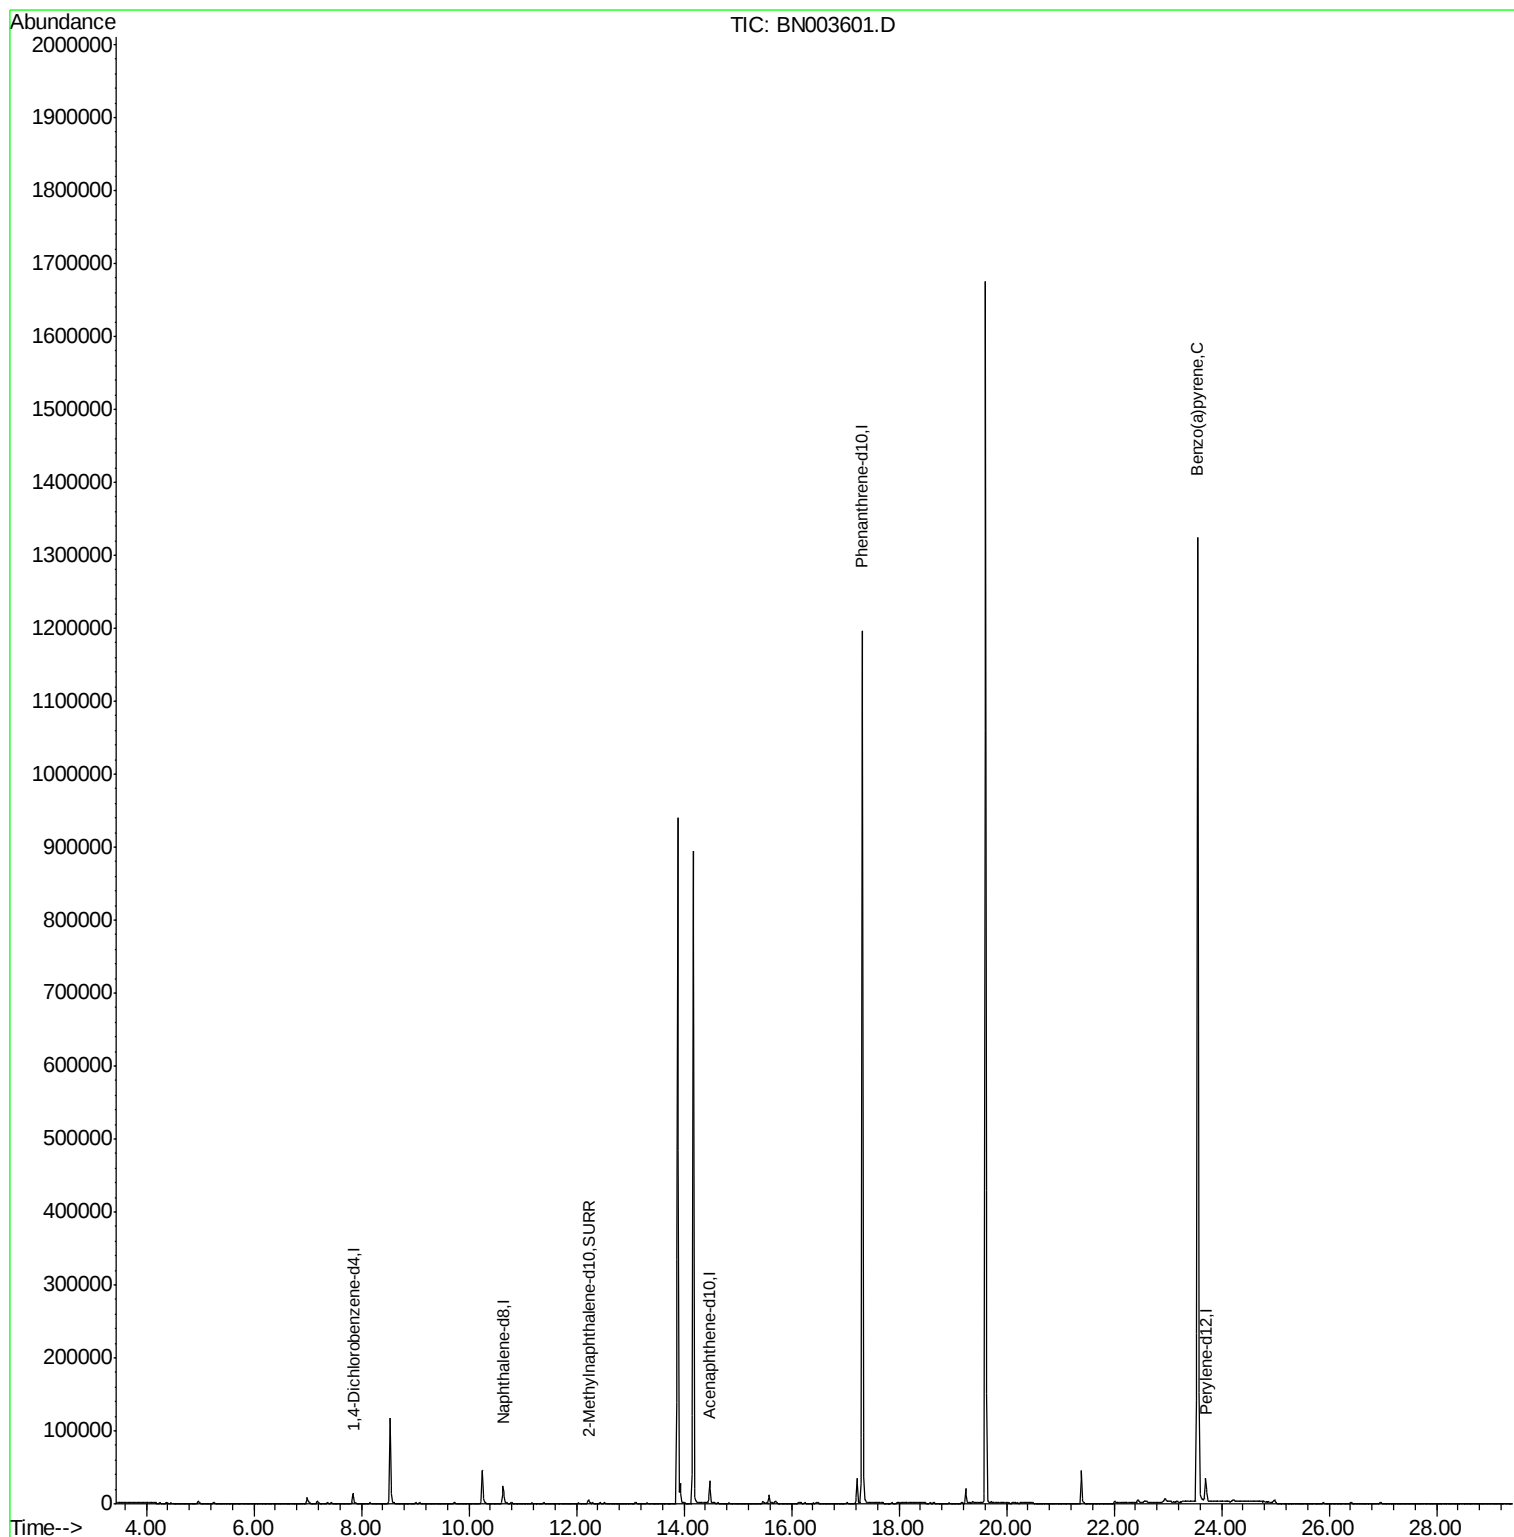

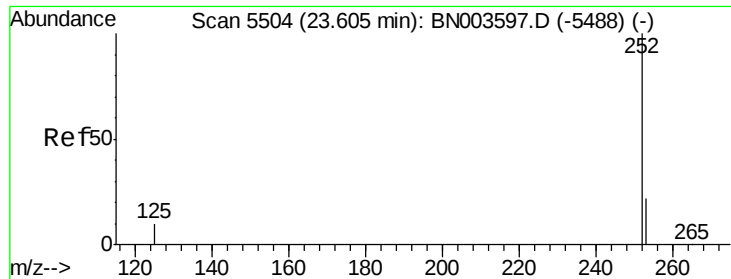

#23

Benzo(a)pyrene

Concen: 0.039 ng/ul

RT: 23.56 min Scan# 5488

Delta R.T. -0.05 min

Lab File: BN003601.D


Acq: 19 Nov 2018 19:16

Instrument :

BNA_N

ClientSampleId :

A40Z4

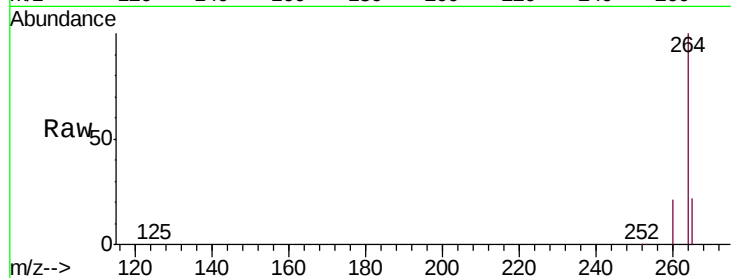

Tgt Ion:	252	Resp:	6635
Ion	Ratio	Lower	Upper
252	100		
253	41.2	19.0	28.4#
125	63.5	10.2	15.4#

