

Data File : BN003605.D
Acq On : 19 Nov 2018 21:36
Operator : MJ/SJ
Sample : J5928-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4102MSD

Quant Time: Nov 20 01:50:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	8759	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	35225	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	17321	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	1740764	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	46467	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	9295	0.17	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	14.54	153	1231569	18.020	ng/ul	98
23) Benzo(a)pyrene	23.56	252	8773	0.053	ng/ul#	20


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003605.D
Acq On : 19 Nov 2018 21:36
Operator : MJ/SJ
Sample : J5928-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4102MSD

Quant Time: Nov 20 01:50:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

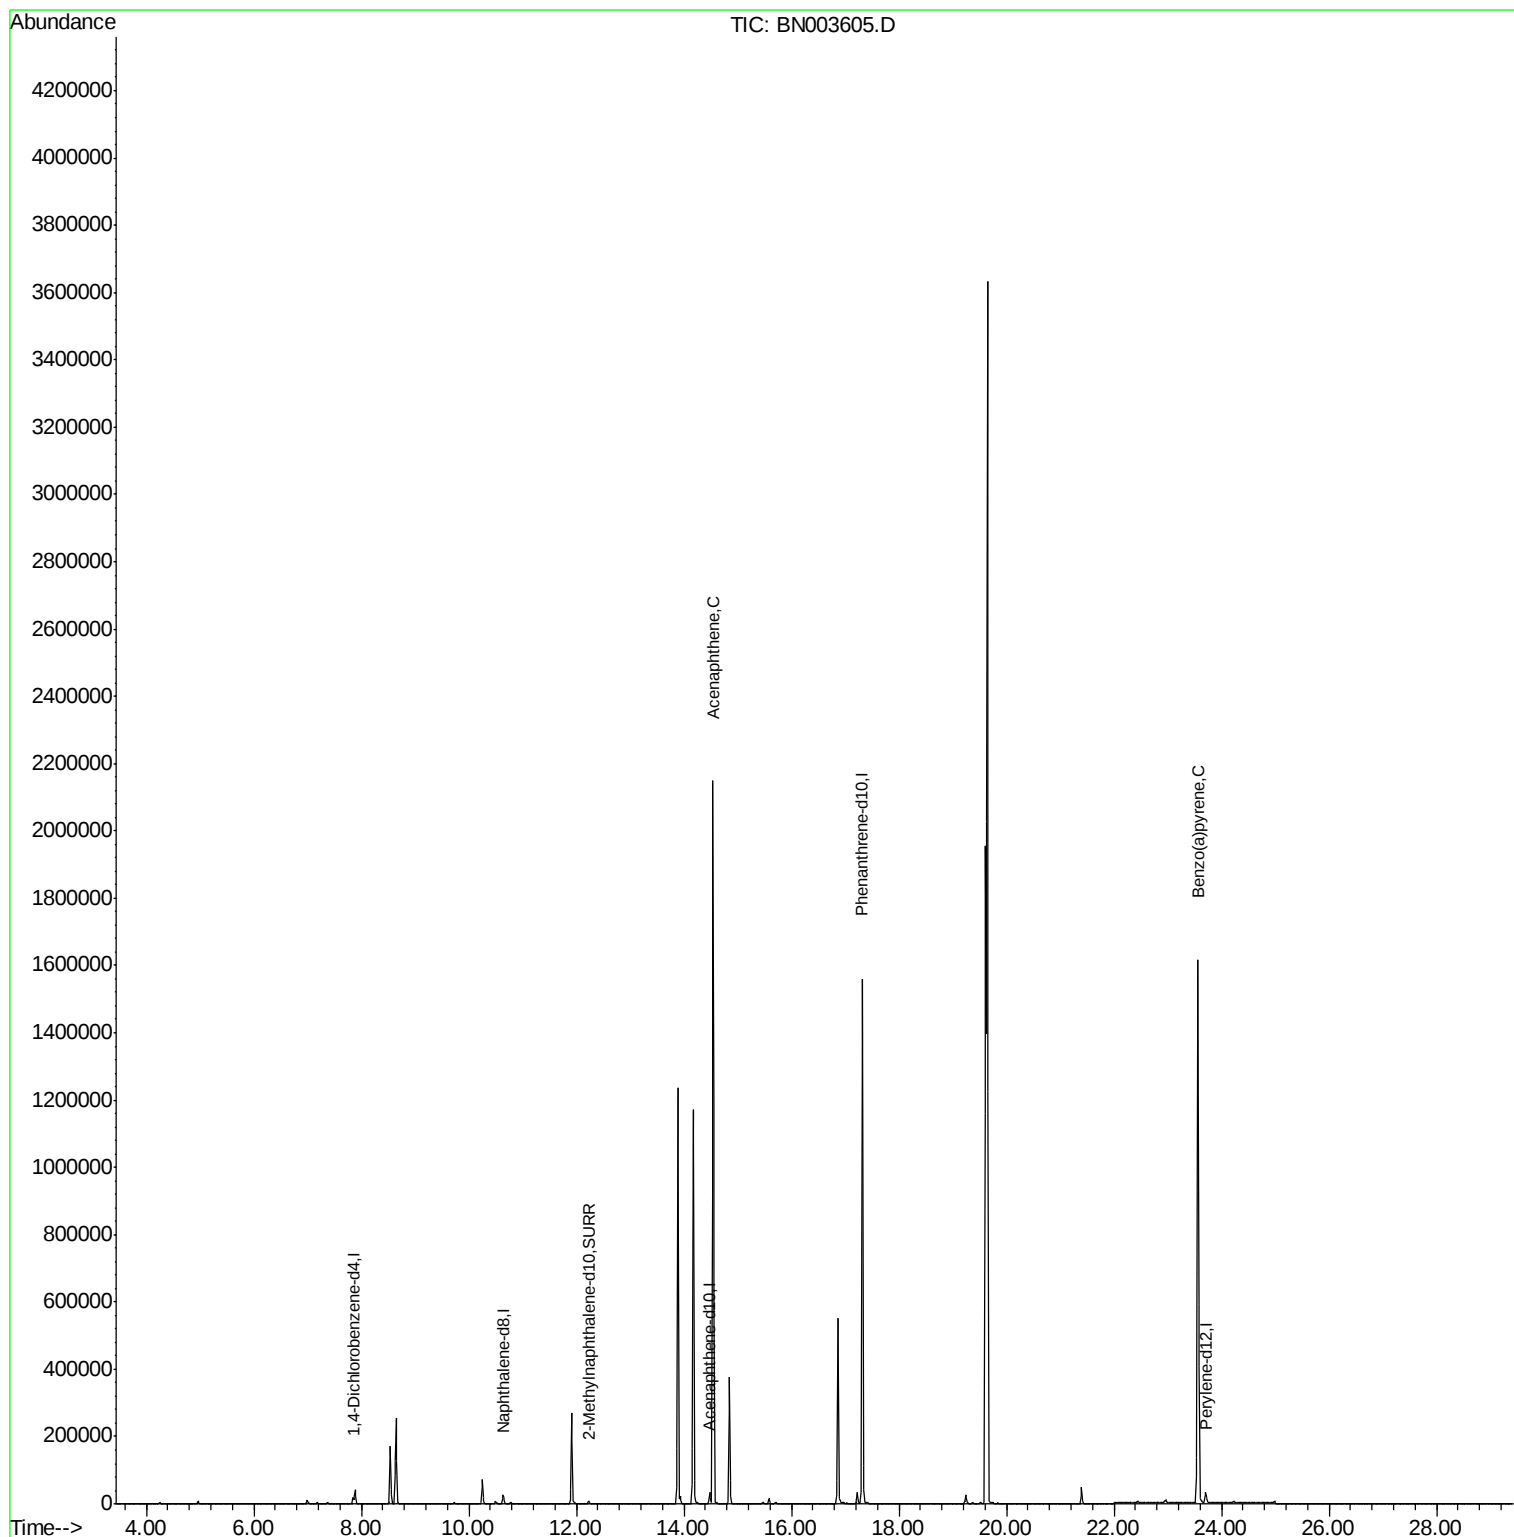

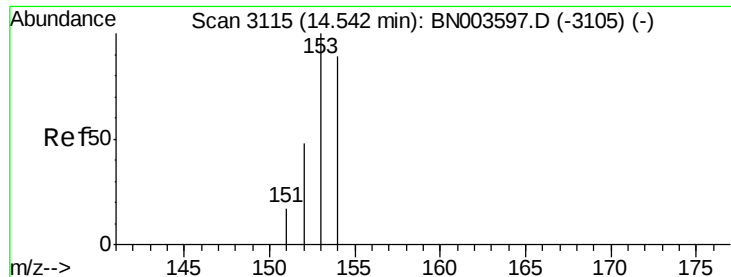

#8

Acenaphthene

Concen: 18.020 ng/ul

RT: 14.54 min Scan# 3115

Delta R.T. -0.00 min

Lab File: BN003605.D

Acq: 19 Nov 2018 21:36

Instrument :

BNA_N

ClientSampleId :

A4102MSD


Tgt Ion:153 Resp: 1231569

Ion Ratio Lower Upper

153 100

152 46.8 39.3 58.9




154 89.4 70.3 105.5

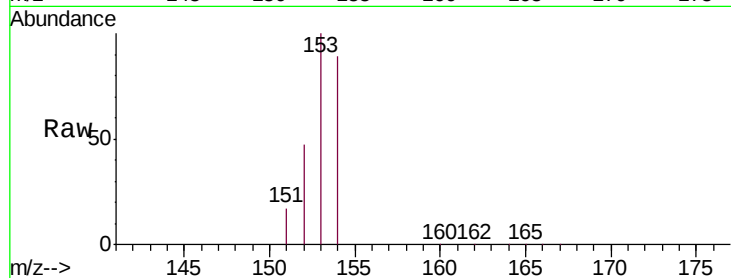

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

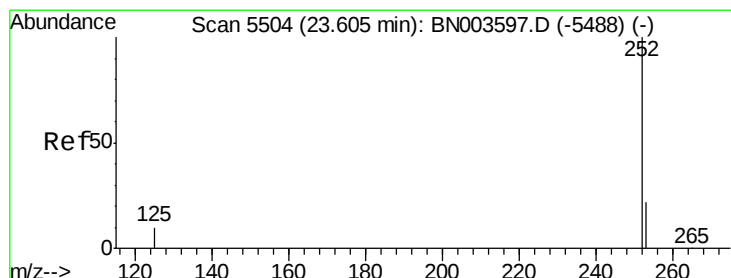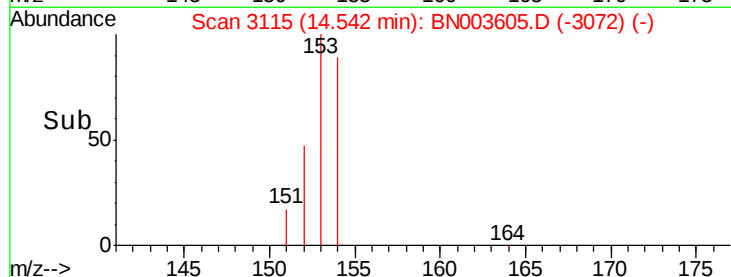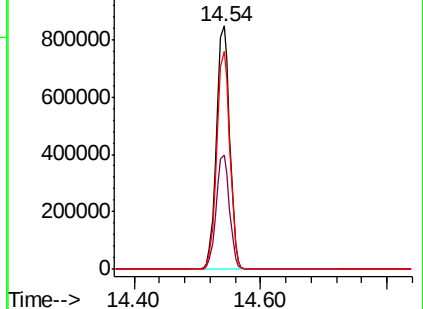

#23

Benzo(a)pyrene

Concen: 0.053 ng/ul

RT: 23.56 min Scan# 5488

Delta R.T. -0.05 min

Lab File: BN003605.D

Acq: 19 Nov 2018 21:36


Tgt Ion:252 Resp: 8773

Ion Ratio Lower Upper

252 100

253 41.5 19.0 28.4#

125 76.7 10.2 15.4#

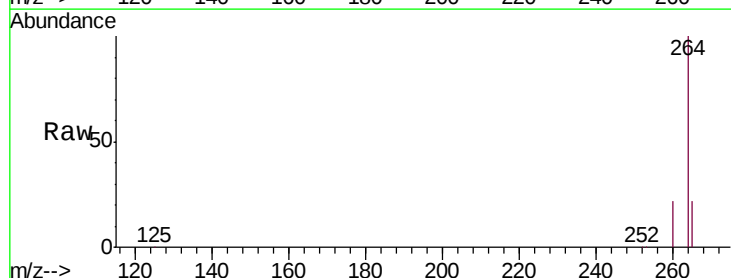

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

