

Data File : BN003609.D
Acq On : 19 Nov 2018 23:56
Operator : MJ/SJ
Sample : J5928-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z0

Quant Time: Nov 20 01:50:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	9420	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	33112	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	19445	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	3264087	0.40	ng/ul	0.10
16) Chrysene-d12	21.52	240	52	0.40	ng/ul	0.13
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.71
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	17780	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Qvalue	
17) Pyrene	19.64	202	2403	12.885	ng/ul#	78
18) Benzo(a)anthracene	21.55	228	108	0.658	ng/ul#	1
19) Chrysene	21.55	228	108	0.575	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003609.D
Acq On : 19 Nov 2018 23:56
Operator : MJ/SJ
Sample : J5928-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Z0

Quant Time: Nov 20 01:50:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 01:46:26 2018
Response via : Initial Calibration

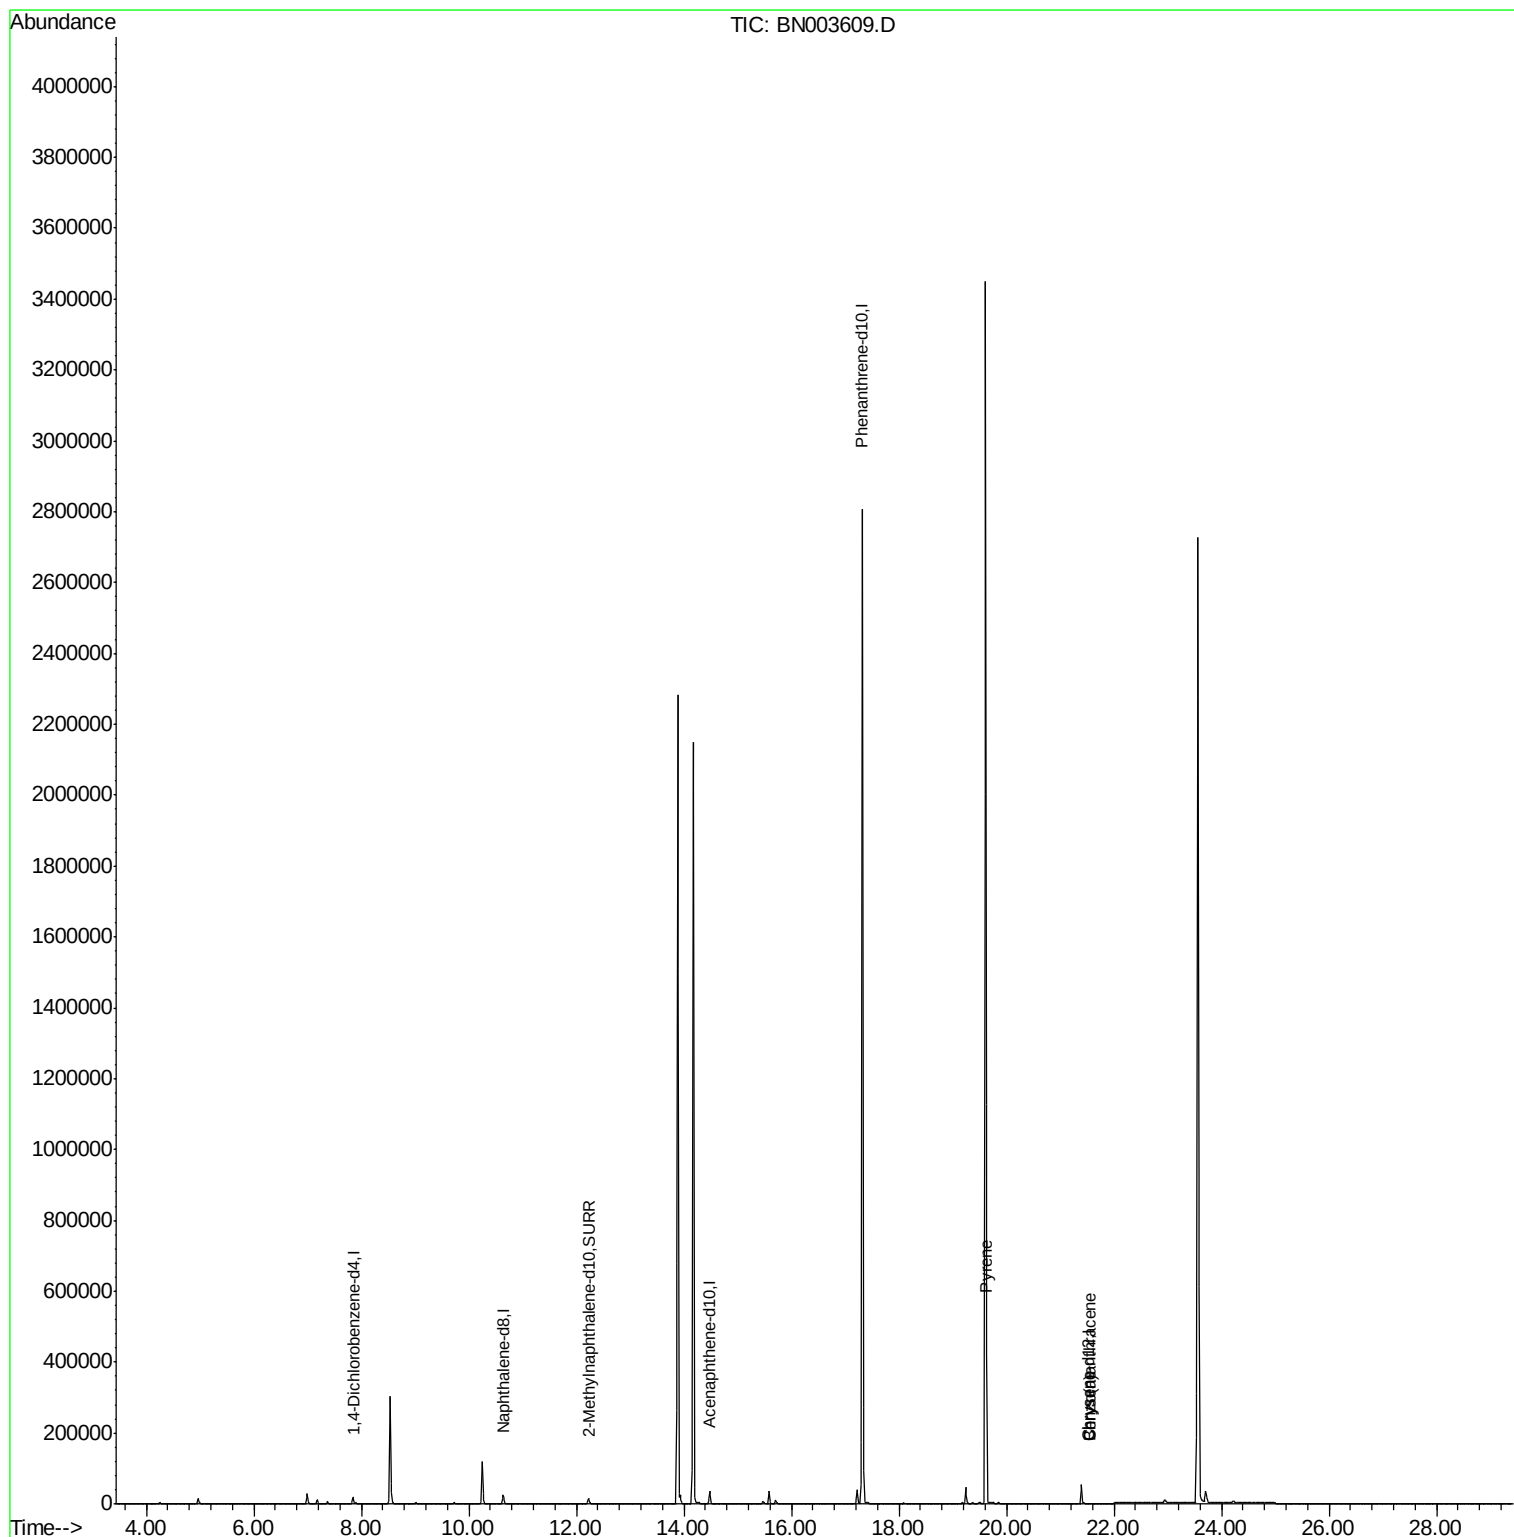

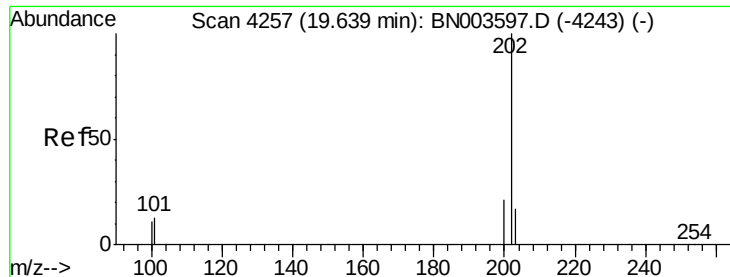

#17

Pyrene

Concen: 12.885 ng/ul

RT: 19.64 min Scan# 4257

Delta R.T. -0.00 min

Lab File: BN003609.D

Acq: 19 Nov 2018 23:56

Instrument :

BNA_N

ClientSampleId :

A40Z0


Tgt Ion:202 Resp: 2403

Ion Ratio Lower Upper

202 100

101 19.7 10.3 15.5#




100 20.8 8.5 12.7#

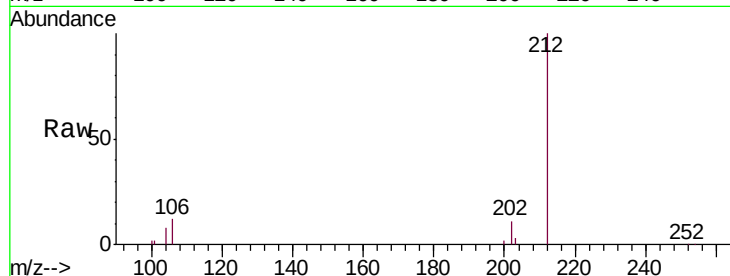

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

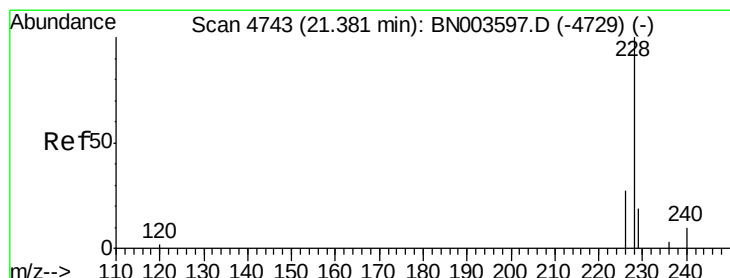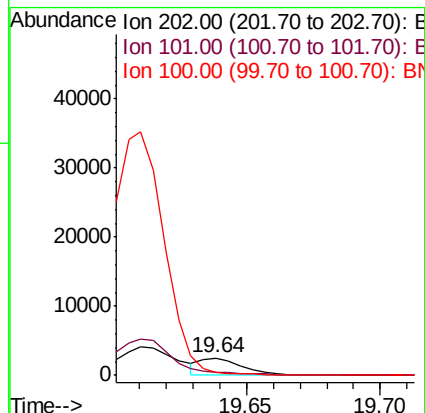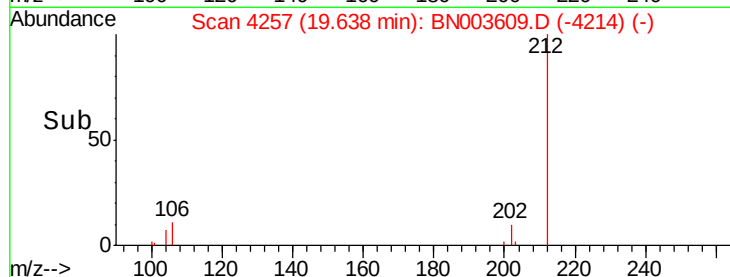

#18

Benzo(a)anthracene

Concen: 0.658 ng/ul

RT: 21.55 min Scan# 4800

Delta R.T. 0.17 min

Lab File: BN003609.D

Acq: 19 Nov 2018 23:56


Tgt Ion:228 Resp: 108

Ion Ratio Lower Upper

228 100

229 98.3 15.6 23.4#



226 98.3 21.1 31.7#



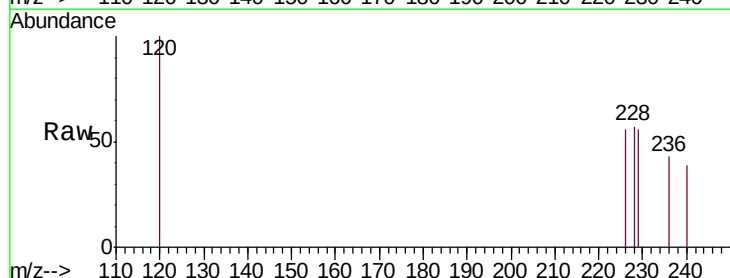


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

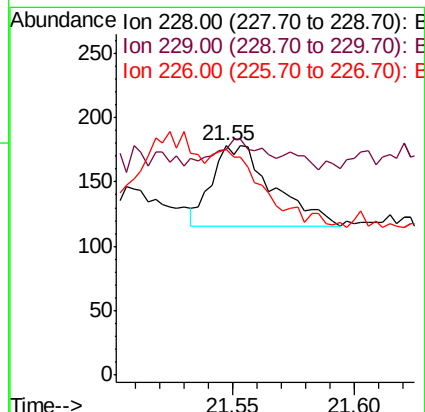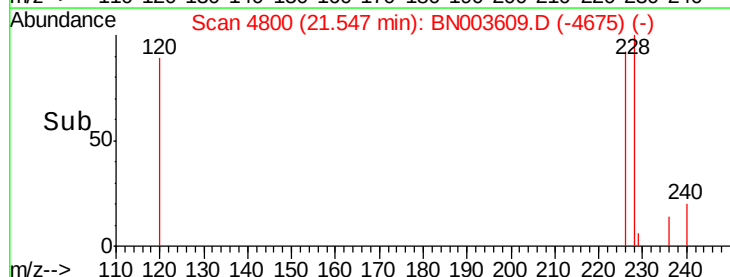

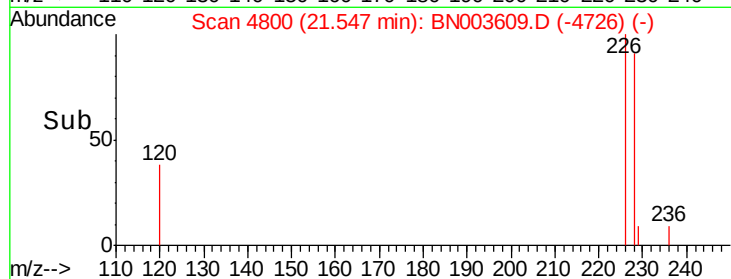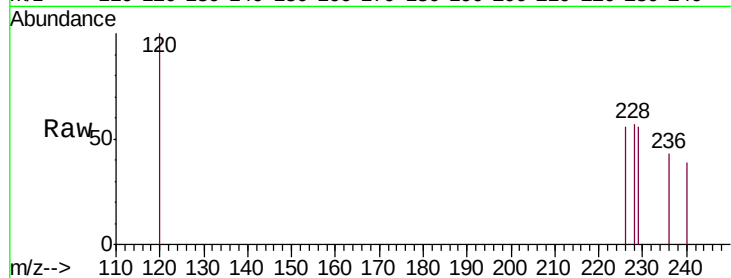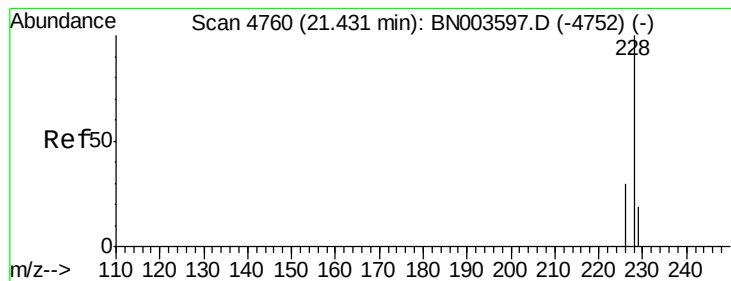

#19

Chrysene

Concen: 0.575 ng/ul

RT: 21.55 min Scan# 4800

Delta R.T. 0.12 min

Lab File: BN003609.D

Acq: 19 Nov 2018 23:56

Instrument :

BNA_N

ClientSampleId :

A40Z0

Tgt Ion:228 Resp: 108

Ion Ratio Lower Upper

228 100

226 98.3 24.0 36.0#

229 98.3 15.7 23.5#

