

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111918\
Quantitation Report (Not Reviewed)

Data File : BN003614.D
Acq On : 20 Nov 2018 02:51
Operator : MJ/SJ
Sample : J5928-21
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y4

Quant Time: Nov 20 03:30:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 03:27:39 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	8239	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	31558	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	18232	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.32	188	2565566	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	40282	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	12973	0.27	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.56	252	9747	0.068	ng/ul#	Qvalue 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003614.D
Acq On : 20 Nov 2018 02:51
Operator : MJ/SJ
Sample : J5928-21
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A40Y4

Quant Time: Nov 20 03:30:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 20 03:27:39 2018
Response via : Initial Calibration

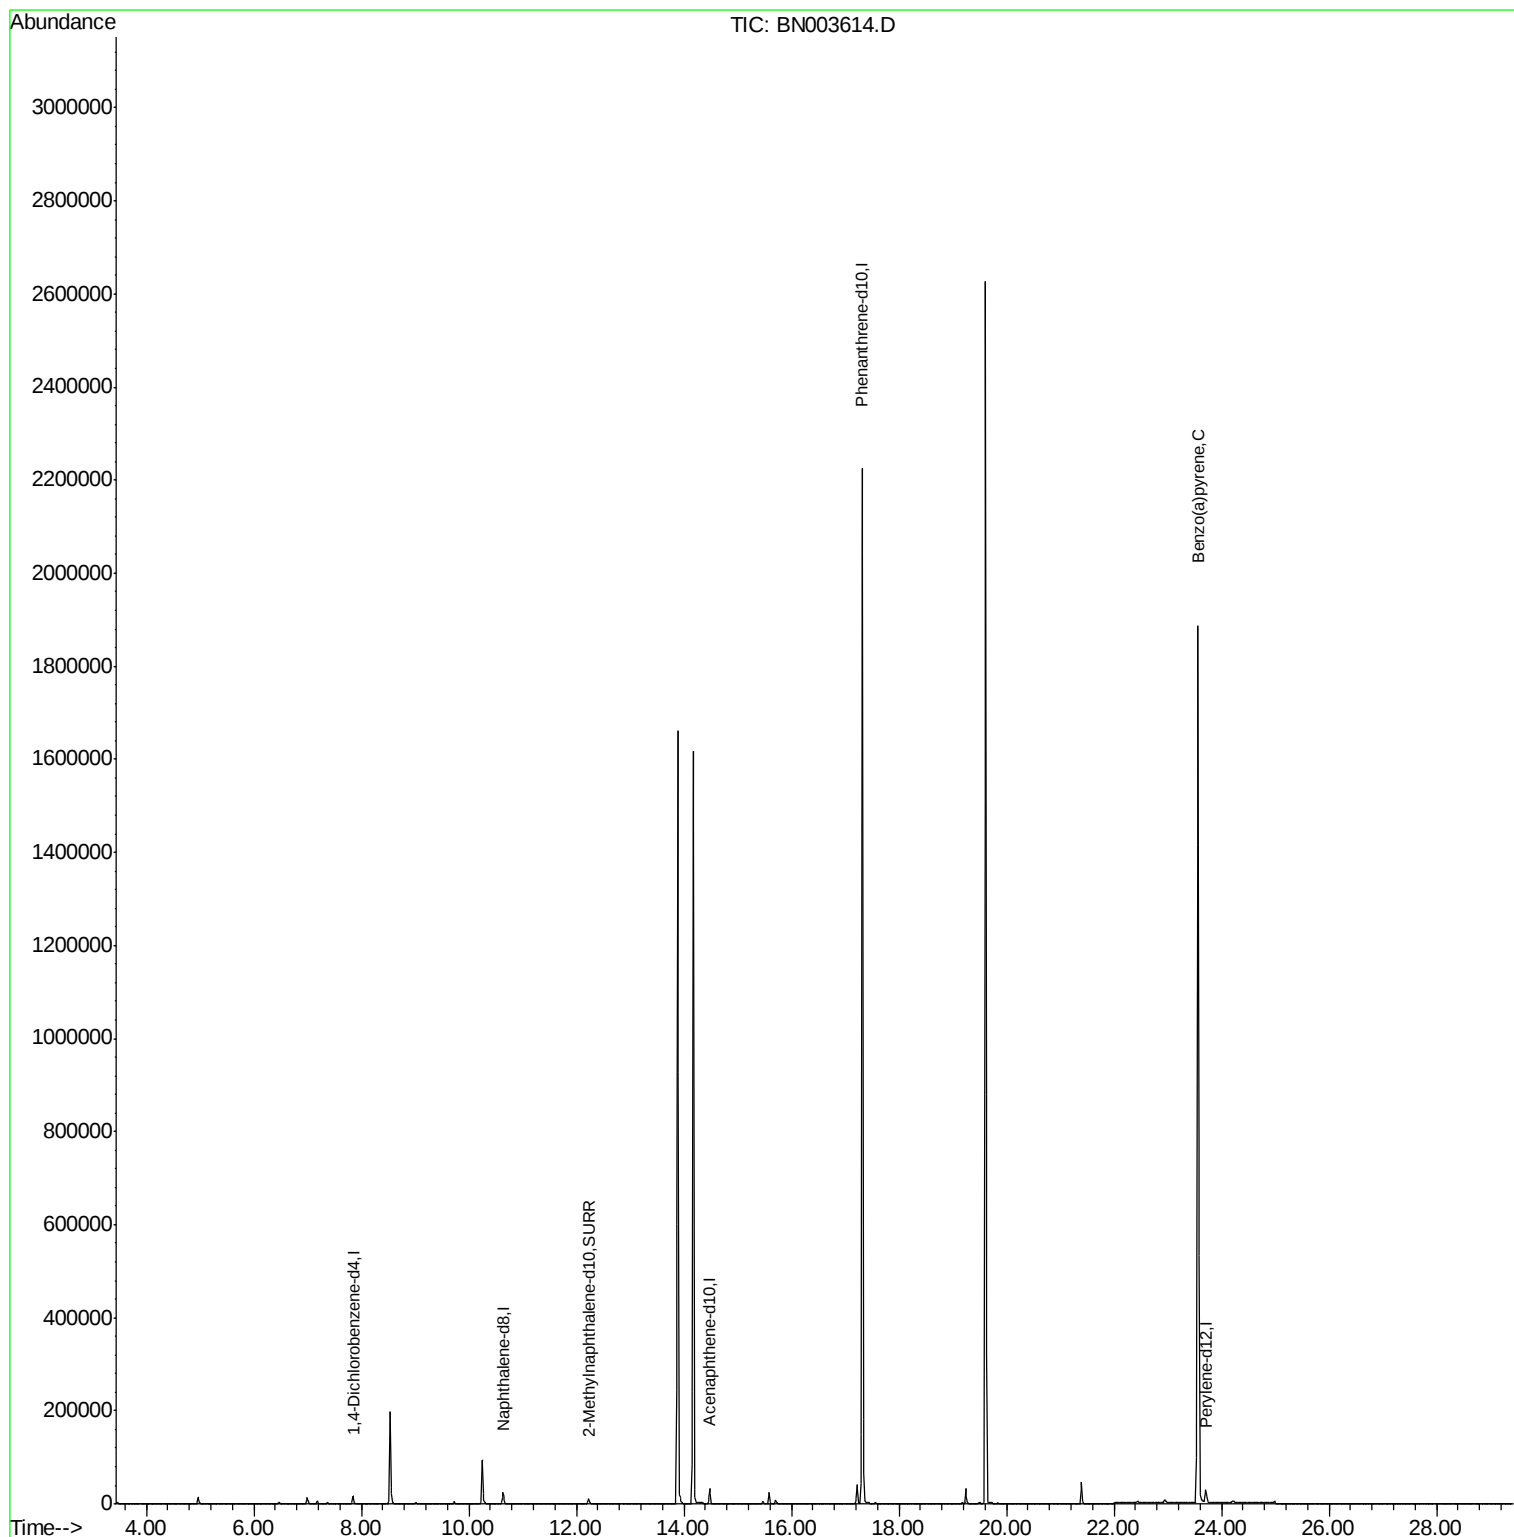

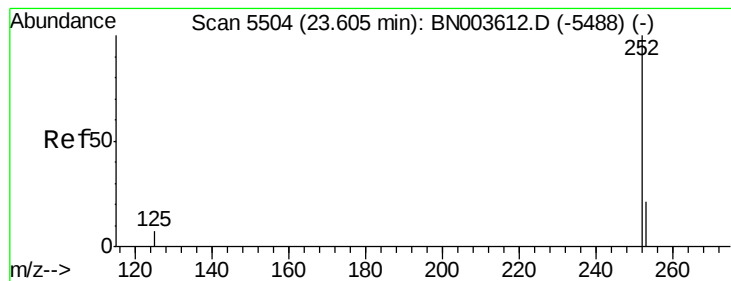

#23

Benzo(a)pyrene

Concen: 0.068 ng/ul

RT: 23.56 min Scan# 5490

Delta R.T. -0.04 min

Lab File: BN003614.D


Acq: 20 Nov 2018 02:51

Instrument :

BNA_N

ClientSampleId :

A40Y4

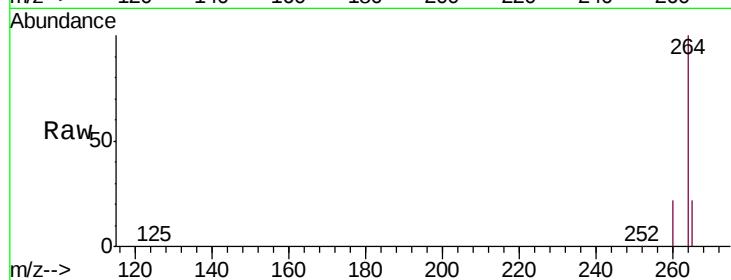


Tgt Ion: 252 Resp: 9747

Ion Ratio Lower Upper

252 100

253 35.2 19.0 28.4#

125 34.2 10.2 15.4#

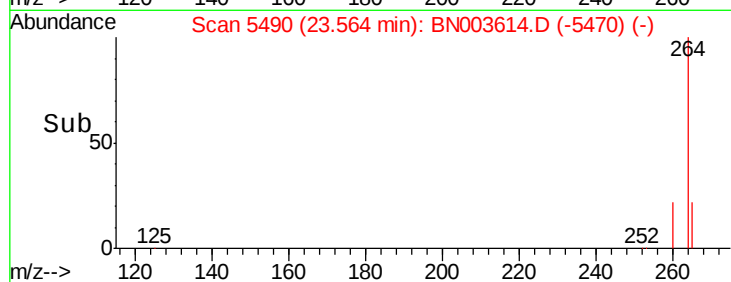

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

